


NJC

Accepted Manuscript



This article can be cited before page numbers have been issued, to do this please use: S. Zhu, C. Lei, Y. Gao, J. Sun, H. Peng, H. Gao, R. Zhang, R. Wang, X. Zhao and H. Wang, *New J. Chem.*, 2018, DOI: 10.1039/C7NJ04574C.

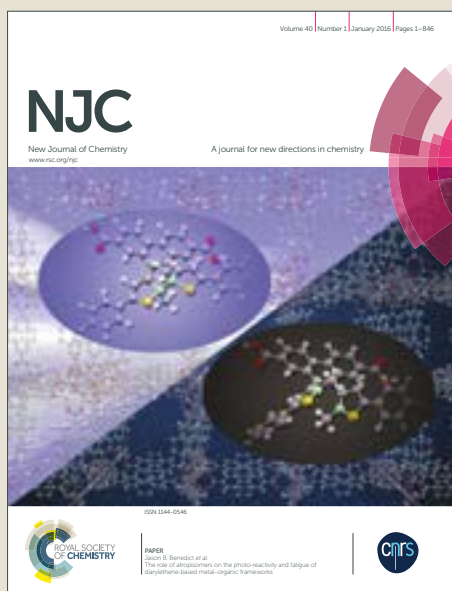

This is an Accepted Manuscript, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this Accepted Manuscript with the edited and formatted Advance Article as soon as it is available.

You can find more information about Accepted Manuscripts in the [author guidelines](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the ethical guidelines, outlined in our [author and reviewer resource centre](#), still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this Accepted Manuscript or any consequences arising from the use of any information it contains.



Journal Name

ARTICLE

A simple and label-free fluorescence detection of ascorbic acid in rat brain microdialysates in the presence of catecholamines

Shuyun Zhu,^{a,b,*†} Cuihua Lei,^{a†} Yue Gao,^a Jing Sun,^b Hongwei Peng,^c Han Gao,^a Ruixue Zhang,^a Rui Wang,^a Xian-En Zhao^{a,b,*} and Hua Wang^{a*}

Received 00th January 20xx,
Accepted 00th January 20xx

DOI: 10.1039/x0xx00000x

www.rsc.org/

Ascorbic acid (AA), as one of the most important neurochemical in cerebral systems, plays a vital role in many physiological and pathological processes. Herein, a facile, label-free, and ultrasensitive fluorescence sensing system was developed for the determination of AA based on the Ag⁺-*o*-phenylenediamine (OPD) interaction. OPD could be oxidized by Ag⁺ to generate fluorescent 2,3-diaminophenazine (OPDox). When AA was introduced, on one hand, AA can inhibit the oxidation process due to its strong reducing capability. On the other hand, AA can be oxidized to dehydro-AA with an absorption peak at 380 nm, which has a good spectral overlap with the emission of OPDox. Thus, the inner filter effect (IFE) between dehydro-AA and OPDox may occur. Therefore, the introduction of AA can intensively suppress the fluorescence of Ag⁺-OPD system. Benefited from the remarkable synergistic effect of reducing capability of AA and IFE, a facile and ultrasensitive sensor was constructed successfully for AA sensing. The whole detection procedure was achieved within 10 min. The linear response range of AA was obtained from 0.05–40 μM with a detection limit of 10 nM. This developed method enjoyed many merits including more simplicity, good selectivity, excellent biocompatibility, and more cost-effective without using any nanomaterials. Notably, the proposed method was successfully applied to detect AA in rat brain microdialysates in the presence of catecholamines, thus providing a new route for AA detection in physiological and pathological fields.

1. Introduction

Monitoring the distribution of reactive species in living systems is of great importance for understanding their physiological functions and pathological effects, as well as early stage diagnosis of some serious diseases. Ascorbic acid (AA) is one of the most important neurochemicals in cerebral systems, which plays a vital role in many physiological and pathological processes.¹ Specifically, AA not only functions as an antioxidant in the intracellular antioxidant system, but also acts as a neuromodulator of both dopamine and glutamate-mediated neurotransmission.^{2–5} Moreover, the level of AA is related to some diseases; for instance, the lack of AA will result in scurvy, and excessive intake of AA can lead to urinary stone, diarrhea, and stomach convulsion.^{6,7} In this regard, the facile and effective measurements of AA in the cerebral neuron system of living animals are of great physiological and

pathological importance and highly desired.^{8,9}

Up to now, some analysis methods have been implemented to detect AA such as electrochemistry,¹⁰ capillary electrophoresis,¹¹ gas chromatography-mass spectrometry,¹² and high-performance liquid chromatography.¹³ Although many approaches were well-established, the sophisticated instrumentation, tedious sample preparation, and separation procedures involved might limit their practical applications. To resolve these problems, Mao's group successfully developed electrochemical methods for in vivo measurement of AA for the first time.¹⁴ Nevertheless, more simple but effective measurement methods for AA in the cerebral systems are still urgently desired.

Fluorescence detection systems are attracting a great deal of interest as a quantitative analytical approach because of their convenient operation, high sensitivity and selectivity, and directly monitoring the target analytes of live cells, tissues, and even animals^{15–17} without a complicated pretreated process and instrumentation during the assay operations. Especially with the development of nanoscience and nanotechnology, various kinds of nanomaterials have been used as fluorescent probes for the determination of AA. For instance, Tang's group designed cobalt oxyhydroxide (CoOOH)-modified persistent luminescent nanoparticles (Sr₂MgSi₂O₇: 1% Eu, 2% Dy) for the determination and screening of AA in living cells and in vivo based on the specific reaction of CoOOH.¹⁸ Lin's group designed Fe³⁺-functionalized carbon quantum dots (CQDs) based on the specific redox reaction between Fe³⁺ and AA for

^a Institute of Medicine and Materials Applied Technologies, College of Chemistry and Chemical Engineering, Qufu Normal University, Qufu City, Shandong Province, 273165, China. E-mail: shuyunzhu1981@163.com (S. Zhu); xianenzhao@163.com (X. Zhao); huawangafnu@126.com (H. Wang).

^b Qinghai Key Laboratory of Qinghai-Tibet Plateau Biological Resources, Northwest Institute of Plateau Biology, Chinese Academy of Sciences, Xining City, Qinghai Province, 810001, Qinghai, China.


^c Hospital of University, Qufu Normal University, Qufu City, Shandong 273165, China.

† The authors contributed equally to this work.

Electronic Supplementary Information (ESI) available: See DOI: 10.1039/x0xx00000x

the detection of AA in rat brain microdialysates.¹⁹ They also synthesized tris(hydroxymethyl)-aminomethane-derived carbon dots (CDs)-modified nanoflakes (tris-derivedCDs-CoOOH) for monitoring cerebral AA in brain microdialysate.²⁰ Although these fluorescent nanoprobe displayed good selectivity and sensitivity for the determination of AA in living cells or microdialysates, they are complicated due to the time-consuming synthesis procedure and complex post treatment process. In addition, the detection of AA in biological matrices may usually suffers from interferences by catecholamines such as dopamine (DA), norepinephrine (NE), L-levodopa (L-DOPA), epinephrine (EP), 5-hydroxytryptamine (5-HT) and so on. Therefore, it is necessary to develop new methods for the determination of AA in the presence of catecholamines with high selectivity and sensitivity.

In this study, for the first time, we reported a rapid, simple, and novel method for the highly sensitive and selective detection of AA in rat brain microdialysates. As shown in Scheme 1, silver ions (Ag^+), as the oxidase mimic, can catalyze the oxidation of *o*-phenylenediamine (OPD) to form 2,3-diaminophenazine (OPDox) showing a strong photoluminescence.^{21,22} AA exhibits high reducing capabilities due to its hexose sugar acid with a γ -lactone structure,²³ which could inhibit the generation of luminescent OPDox. Moreover, there is a good spectral overlap between the absorption spectra of the yielding dehydro-AA and the emission spectra of OPDox, thus leading to the inner filter effect (IFE). Therefore, the introduction of AA could result in the remarkable decrease of the fluorescence intensity of Ag^+ -OPD system. Based on these facts, a simple and label-free fluorescent method has thus been developed for the detection of AA without the preparation of nanomaterials and the use of expensive instruments. Subsequently, the developed method was successfully applied to the direct analysis of AA in rat brain microdialysates.

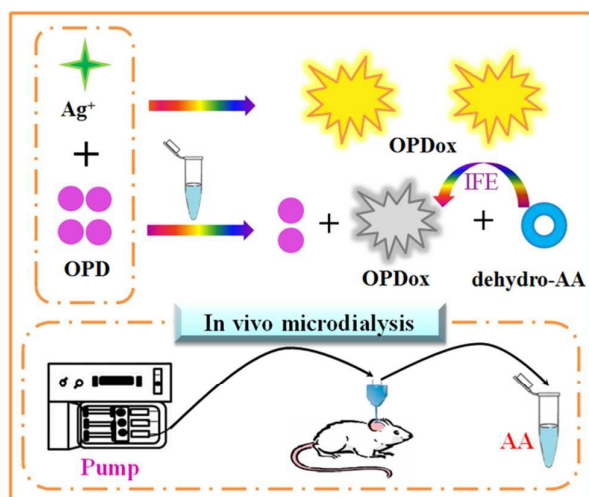

Scheme 1 Schematic illustration of the strategy of facile ascorbic acid sensing.

2. Experimental

2.1 Reagents

Ascorbic acid (AA), dopamine (DA), AgNO_3 , *o*-phenylenediamine (OPD), hydrogen peroxide (H_2O_2), ethylene diamine tetraacetic acid (EDTA), $\text{Na}_2\text{HPO}_4 \cdot 12\text{H}_2\text{O}$, and $\text{NaH}_2\text{PO}_4 \cdot 2\text{H}_2\text{O}$ were purchased from Aladdin Company (Shanghai, China). The uric acid (UA), tyrosine (Tyr), serine (Ser), glutamic acid (Glu), lysine (Lys), phenylalanine (Phe), arginine (Arg), glycine (Gly), epinephrine (EP), norepinephrine (NE), levodopa (L-DOPA), dopamine (DA), 5-hydroxytryptamine (5-HT), glutathione (GSH), homocysteine (Hcy), Cysteine (Cys), and glucose were purchased from Alfa Aesar. Reduced *N*-ethylmaleimide (NEM) was purchased from Sigma-Aldrich. 10 mM phosphate buffer solutions (PBS) were prepared by mixing stock standard solutions of Na_2HPO_4 and NaH_2PO_4 . All reagents were of analytical reagent grade, and used as received. Doubly deionized water was used throughout.

2.2 Apparatus

All fluorescence measurements were carried out on an F-7000 spectrometer (Hitachi, Japan) operated at an excitation wavelength at 417 nm. UV-vis spectra were recorded on a UV-vis spectrophotometer (Shimadzu, UV-3600, Japan). In vivo microdialysis sampling was accomplished by using a CMA 402 Syringe Pump (CMA, Solna, Sweden), a CMA 120 System (CMA, Solna, Sweden) for freely moving animals, a microdialysis MAB6 probe (Stockholm, Sweden) which was perfused with Ringer's solution (5 mM) at a flow rate of 2.0 $\mu\text{L}/\text{min}$, and ASI stereotaxic flat skull coordinates (ASI Instruments Inc., MI, USA).

2.3 Procedure for AA detection

For the detection of AA, 15 μL of 6 mM OPD were diluted in 472 μL of PBS buffer (10 mM, pH 7.0), followed by the addition of 8 μL of 6 mM AgNO_3 , and then 5 μL of different concentrations of AA. The samples were incubated for 10 min in dark at room temperature before fluorescence measurement. The selectivity of AA was explored in a similar way by adding other interferences. The fluorescence spectra were collected under excitation at 417 nm, and the slit wavelengths of both excitation and emission were 5 nm, respectively.

2.4. Detection of AA in rat brain microdialysates

In vivo microdialysis experiments were performed as our previous work.^{24,25} Briefly, the rats were anesthetized with 20% urethane (1.2 g/kg, i.p.) before probe implantation surgery, and remained anesthetized throughout the experimental period. The rat's body temperature was maintained at 37 $^\circ\text{C}$ during the experimental procedure. A pretreated probe was inserted into the right striatum with stereotaxic flat skull coordinates: A: + 1.0 mm from bregma, L: \pm 2.9 mm from midline and H: -3.5 mm from dura. Animals were awake and freely moving with access to food and water throughout the experiment. Next, the brain microdialysis

probe (MAB6) was perfused with artificial cerebrospinal fluid (a CSF) (126 mM of NaCl, 27.5 of mM NaHCO₃, 2.4 mM of KCl, 1.1 mM of CaCl₂, 0.85 mM of MgCl₂, 0.5 mM of Na₂SO₄, 0.5 mM of KH₂PO₄, pH =7.0) at a rate of 2.0 μL/min using a microinjection pump (CMA 402, Sweden) and microsyringe (CMA, 1.0 mL) for 90 min to reach baseline values. Finally, every 50 μL of microdialysate was collected for the following AA sensing.

3. Results and discussion

3.1. Design and establishment of AA sensing system

As shown in Fig. 1, the aqueous solution of OPD has always remained colorless and exhibited negligible fluorescence (curve and vial 1). In contrast, the introduction of Ag⁺ essentially triggers the oxidative reaction of OPD, during which the original colorless and non-fluorescent solution gradually turned to pale yellow in color and showed intense orange-yellow fluorescence under ultraviolet (curve and vial 2). As shown in Fig. 1A, the Ag⁺-OPD mixed solution has an obvious absorption peak at about 417 nm, which belongs to the characteristic absorption spectrum of OPDox, the main oxidation product of OPD.²⁶ Meanwhile, the corresponding emission spectrum in Fig. 1B exhibited a peak at about 557 nm, which is similar to that of OPDox in previous work as well.^{27,28} Then, both the absorption intensity at 417 nm and the fluorescence intensity at 557 nm decreased obviously after the addition of AA (curve and vial 3).

In order to verify the sensing mechanism, the addition sequence of AA was investigated. As shown in Fig. S1, Ag⁺ could oxidize OPD to generate OPDox with a strong fluorescence (curve a). According to the previous report,²¹ Ag⁺ was reduced to zero-valent silver and formed silver nanoparticles (AgNPs). Actually, the formed nanoparticles were observed on a membrane layer by TEM analysis (Fig. S2A). To confirm the components that might comprise such nanoparticles, the thus-formed nanoparticles were characterized by energy-dispersive spectroscopy (EDS) analysis. As shown in Fig. S3, the element comprised in the nanoparticles was silver. These results indicated the formation of AgNPs could occur during the reaction of Ag⁺ and OPD. After AA was added into the Ag⁺-OPD mixed solution, the fluorescence intensity of the solution decreased remarkably (curve b), indicating AA could reduce fluorescent OPDox into non-fluorescent OPD. It has also been reported that AA was common reducing agent for the synthesis of AgNPs.²⁹ So, AA was reacted firstly with Ag⁺ for 5 min followed by the addition of OPD. As shown in curve c of Fig. 1S, the fluorescence intensity of the solution decreased furtherly. Moreover, the formed AgNPs exhibited different size and morphology (Fig. S2B). The results indicated that AA was also responsive to Ag⁺. Therefore, the presence of AA inhibited the generation of OPDox due to its strong reducibility towards both OPDox and Ag⁺. More interestingly, a new absorption peak generated at 380 nm from the yielding dehydro-AA had a good overlap with excitation spectrum of fluorescent OPDox (Fig. S4), resulting in

the occurrence of inner filter effect (IFE). Ascribed to the two reasons, the significant enhancement in the fluorescence along with the oxidative reaction of OPD could be partially suppressed in the presence of AA.

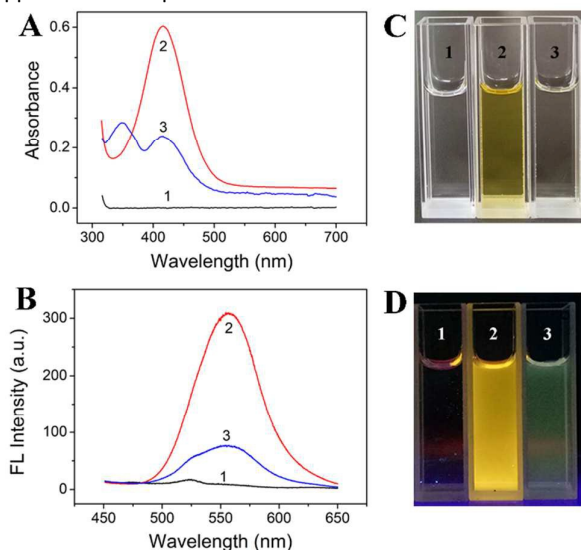


Fig. 1 Absorbance (A) and fluorescence emission spectra (B) of the OPD (1), OPD + Ag⁺ (2), and OPD + Ag⁺ + AA in PBS buffer at pH 7.0. The corresponding photographs under visible (C) and ultraviolet light (D). The final concentrations of OPD, Ag⁺, and AA are 180 μM, 96 μM, and 30 μM, respectively.

Catecholamines, as common interferences, usually coexist in the biological fluids with AA. Therefore, we investigated the influences of catecholamines including DA, EP, NE, L-DOPA, and 5-HT on the fluorescence responses of Ag⁺-OPD system. As shown in Fig. S5, the fluorescence intensity decreases up to 80% at 30 μM AA. In contrast, the presence of 30 μM catecholamines resulted in fluorescence quenching less than 20%. Similarly, the decrease degrees of absorption intensity at 417 nm in the presence of catecholamines were less than that of AA. Besides, no new absorption peak was observed after the addition of catecholamines. These results indicated AA possesses higher inhibition ability for the fluorescence intensity of Ag⁺-OPD system due to the synergistic effect of stronger reducibility of AA and the IFE. Therefore, a convenient fluorimetric assay could be designed for sensing AA sensitively and selectively.

3.2. Optimization of the sensing system

The reaction conditions were optimized to establish the optimum analytical conditions. pH is a crucial factor for almost every sensing system. Fig. 2A shows the fluorescence intensity of Ag⁺-OPD system in the presence and absence of AA under the media of different pH values. The fluorescence intensity showed the largest difference when the pH was around 7.0. In the strong acidic medium, the amino groups of OPD could be protonated, which could inhibit the oxidation by Ag⁺. When the pH value was higher than 7.0, Ag⁺ might be more prone to hydrolysis, which could decrease its oxidization ability.

ARTICLE

Journal Name

Moreover, the pH 7.0 was established to fit for enzyme mimetic reaction. Therefore, pH 7.0 was the optimal condition for the sensing system.

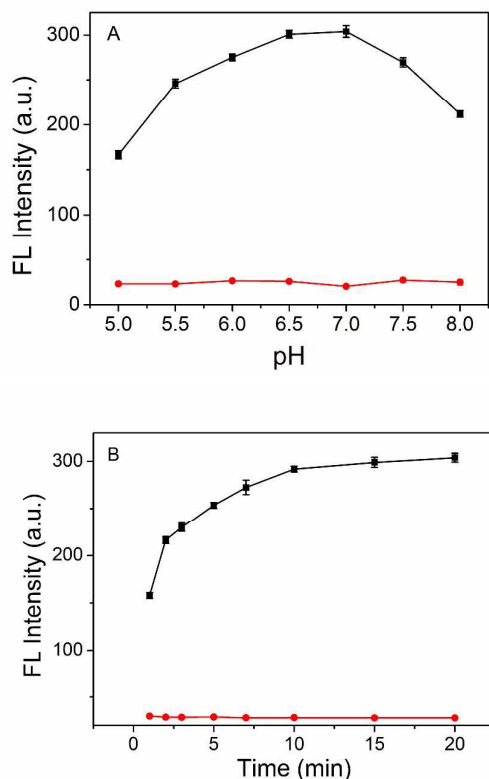


Fig. 2 Effect of pH (A) and reaction time (B) on the fluorescence intensity at 557 nm in the absence (■) and presence (●) of 40 μM AA. Other conditions are the same as that in the Fig. 1.

The effect of reaction time on the detection of AA was also studied, and the experimental results were shown in Fig. 2B. The results indicated that the fluorescence of Ag^+ -OPD system increased gradually and reached about 90% of the maximum when the reaction time reached 10 min, showing that the oxidation reaction was almost complete in 10 min. While in the presence of AA, the fluorescence decreased quickly in the first 1 min, and then remained almost constant in the following 20 min. Thus, the optimum time for the proposed system was set as 10 min.

3.3. Sensitivity of the sensing system

Under the optimization conditions, we evaluated the analysis capability of this system for the quantitative detection of AA. As shown in Fig. 3A, it was clearly seen that with the increase of AA concentrations, the fluorescence intensities of Ag^+ -OPD system decreased gradually while the $\Delta F = F_0 - F$ increased systematically, where F_0 and F are fluorescence intensities at 557 nm in the absence and presence of AA, respectively. The ΔF exhibited a good linear relationship with AA in the two

concentration ranges of 0.05–1.0 μM and 1.0–40 μM. The regression equations were $\Delta F = 13.88 + 28.39 C_{\text{AA}} (\mu\text{M})$ ($R^2=0.995$) and $\Delta F = 42.56 + 6.147 C_{\text{AA}} (\mu\text{M})$ ($R^2=0.997$), respectively. The detection limit can reach as low as 10 nM estimated by a signal to noise of 3. Moreover, the analysis repeatability of the proposed method was evaluated by six repeated measurements of 0.5 μM and 5.0 μM AA and the relative standard deviation (RSD) was 3.61% and 2.37%, respectively, demonstrating the reliability of the proposed method.

In addition, we compared the characteristics of the proposed sensor with other fluorescent AA sensors reported elsewhere. As shown in Table 1, this proposed system could provide better detection sensitivity in comparison with those of other fluorescent nanoprobes including gold nanoclusters,³⁰ carbon quantum dots (CQDs),³¹ graphitic carbon nitride nanosheets,³² copper nanoclusters,³³ and graphene quantum dots (GQDs).²³ Moreover, this developed fluorimetric method is relatively simple and fast, of which the whole detection procedure can be finished within 10 min. In contrast, the fluorescent nanomaterials may entail much longer reaction time to prepare by using the complicated synthesis and post-treatment process.

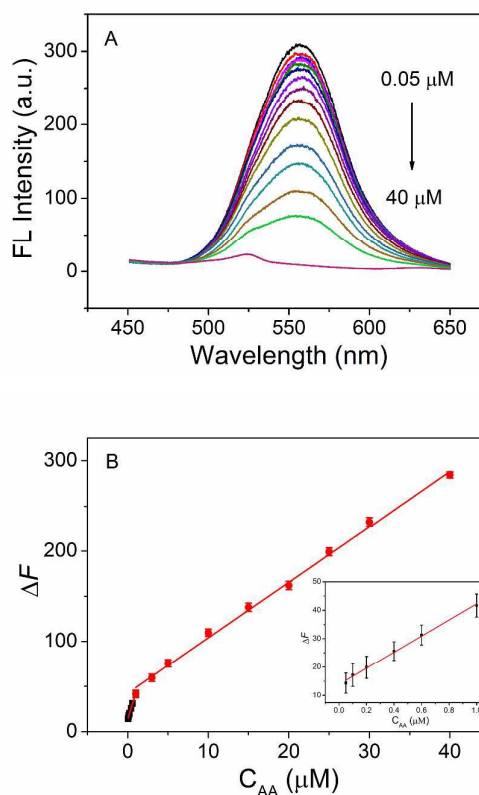


Fig. 3 (A) Fluorescence spectra of the Ag^+ -OPD solution in the presence of varied concentrations of AA (0–40 μM). (B) Relationship between ΔF and the concentrations of AA. Inset: relationship between ΔF and the lower concentrations of AA.

Table 1 Comparison of the detection performances for AA among different probes.

Probes/Ref.	Linear range (μM)	Detection limit (μM)	Synthesis time for probes
Protein-modified Au nanoclusters/[30]	1.5-10	0.2	24 h
Phosphorus/nitrogen dual-doped CQDs ^a /[31]	5-200	1.35	72 h
Graphitic carbon nitride nanosheets/[32]	0.5-200	0.13	24 h
Cu nanoclusters/[33]	0.5-10	0.11	6 h
GQDs ^b /[23]	0.5-250	0.28	28 h
Hexagonal cobalt oxyhydroxide-carbon dots/[34]	0.1-20	0.05	40 min
CdS QDs/[35]	0.06-0.3 1.0-40	0.002	1 h
Ag ⁺ -OPD/ This work	0.05-1.0 1.0-40	0.01	10 min

^a carbon quantum dots^b graphene quantum dots

3.4. Selectivity of Ag⁺-OPD system with different ions and biological molecules

To evaluate the specificity of the developed assay for AA, several potential interfering compounds were investigated under the same conditions. Firstly, various metal ions including K⁺, Ca²⁺, Zn²⁺, Mg²⁺, Na⁺, Mn²⁺, Ba²⁺, Co²⁺, and Cu²⁺ containing Ag⁺-OPD system were measured under 417 nm excitation. As demonstrated in Fig. 4A, these potential metal ions caused no significant signal fluctuations, indicating they showed negligible influence on the fluorescence intensity of Ag⁺-OPD system.

Usually the concentration of catecholamines in biological fluids are much lower than that of AA. Thus, the selectivity of Ag⁺-OPD system was further validated by comparing the signal changes of samples containing the lower concentrations of catecholamines and other common biological molecules. As shown in Fig. 4B, except for GSH, Hcy, and Cys, the response of Ag⁺-OPD system was selective toward AA. Because GSH, Hcy, and Cys could also have somewhat reducing abilities towards Ag⁺, their addition resulted in the decrease of the fluorescence. However, *N*-ethylmaleimide (NEM), a scavenger that can exclusively react with sulfhydryl compound, could effectively eliminate the interference.³⁶ As can be seen from Fig. 4B, after incubation of GSH, Hcy, or Cys with NEM, the Ag⁺-OPD system did not generate obvious fluorescence decrease, whereas the determination of AA was not affected by the introduction of NEM. Therefore, the Ag⁺-OPD system could present a sensitive and selective fluorescent approach toward

AA sensing by employing NEM as an effective GSH, Hcy, and Cys scavenger.

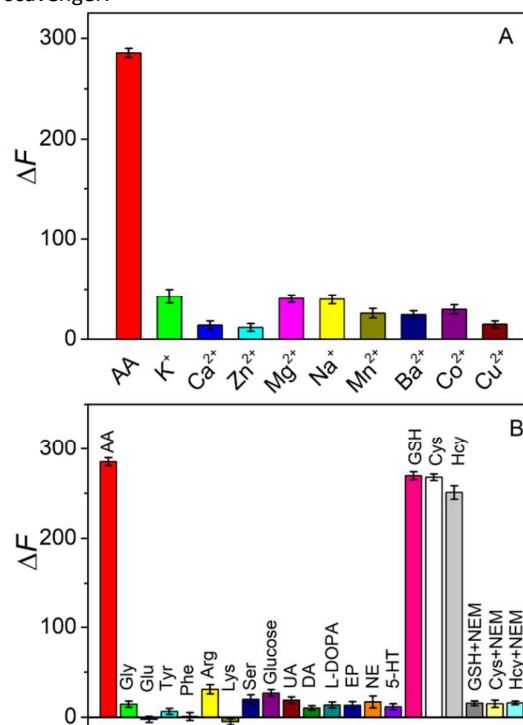


Fig. 4 (A) The selectivity of Ag⁺-OPD system towards different metal ions. The concentration of AA is 40 μM , and the concentration of all the metal ions are 400 μM . **(B)** The selectivity of Ag⁺-OPD system towards other biological molecules. The concentration of AA is 40 μM , and the concentrations of UA, DA, L-DOPA, NE, and EP are 5 μM , respectively. The concentrations of other interfering species are 40 μM . The NEM concentration is 0.3 mM.

3.5. Application of the proposed sensing system to rat brain microdialysates analysis

Recently, AA has been proven to be a kind of neuro molecules, thus monitoring the levels of AA in brain microdialysates are important for the research of physiology, pathology, and clinics. In our experiment, an unknown amount of AA in a rat brain microdialysis sample was estimated by using the standard addition method with 0.5 μM AA solution. As shown in Fig. 5, the fluorescence spectra of Ag⁺-OPD system were recorded in the absence (a) and presence of 50 μL rat brain microdialysates (b). Next, 5 μL 50 μM AA standard solution was added twice (curve c and d, Fig. 5). According to the standard method, the concentration of AA was calculated to be 5.96 μM in the rat brain microdialysates, which is consistent with the previous reports.³⁷

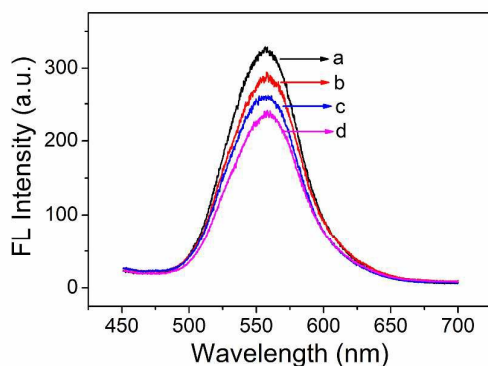


Fig. 5 Fluorescence spectra of Ag^+ -OPD system for AA detection in rat brain microdialysates: Ag^+ -OPD system (a); the successive addition of 50 μL microdialysates (b), 5 μL AA solution (c), and 5 μL AA solution (d).

4. Conclusions

In summary, a novel fluorescent assay was developed for the facile detection of AA based on the synergistic effect of reducing ability of AA and IFE. The Ag^+ -OPD probing system features some excellent chemical properties such as high water solubility and strong fluorescence intensity, which could be served as a novel fluorescence probe for AA sensing. Moreover, no nanomaterials participated in the assays, making it a simple, cost-effective, fast, and lowly laborious candidate. More importantly, this fluorimetric method was successfully applied to the determination of AA in rat brain microdialysates samples, providing a potential platform for AA monitoring from many other biological samples.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements


This work is kindly supported by the National Natural Science Foundation of China (Nos. 21405094, 21775088, and 21675099), the Open Funds of the State Key Laboratory of Electroanalytical Chemistry (No. SKLEAC201506), the Natural Science Foundation of Qinghai Province (2016-ZJ-955), the Development Project of Qinghai Key Laboratory (No. 2017-ZJ-Y10), the National Undergraduate Research Training Program (No. 201610446033, 2017A029), and the Scientific Research Foundation of Qufu Normal University (No. BSQD201203).

Notes and references

- 1 Y. Li and X. Lin, *Sens. Actuators B: Chem.*, 2006, **115**, 134.
- 2 X. Gao, P. Yu, Y. Wang, T. Ohsaka, J. Ye and L. Q. Mao, *Anal. Chem.*, 2013, **85**, 7599.

- 3 K. Liu, P. Yu, Y. Wang, T. Ohsaka and L. Q. Mao, *Anal. Chem.*, 2013, **85**, 9947.
- 4 Y. Lin, P. Yu, J. Hao, Y. Wang, T. Ohsaka and L. Q. Mao, *Anal. Chem.*, 2014, **86**, 3895.
- 5 M. E. Rice, *Trends Neurosci.*, 2000, **23**, 209.
- 6 S. J. Padayatty, A. Katz, Y. Wang, P. Eck, O. Kwon, J. H. Lee, S. Chen, C. Corpe, A. Dutta, S. K. Dutta and M. Levine, *Am. J. Coll. Nutr.*, 2003, **22**, 18.
- 7 M. Sönmeza, G. Türk and A. Yüce, *Theriogenology*, 2005, **63**, 2063.
- 8 T. Finkel and N. J. Holbrook, *Nature*, 2000, **408**, 239.
- 9 M. E. Rice, *Trends Neurosci.*, 2000, **23**, 209.
- 10 S. Y. Zhu, H. J. Li, W. X. Niu and G. B. Xu, *Biosensor. Bioelectron.*, 2009, **25**, 940.
- 11 N. B. Saari, A. Osman, J. Selamat and S. Fujita, *Food Chem.*, 1999, **66**, 57.
- 12 W. D. Mark, B. Guy and V. M. Marc, *Anal. Biochem.*, 1996, **239**, 8.
- 13 M. Yuta, Y. Mayumi, Y. Toshihide, M. Fumiya and Y. Kenichi, *Free Radic. Biol. Med.*, 2012, **53**, 2112.
- 14 M. Zhang, K. Liu, L. Xiang, Y. Lin, L. Su and L. Mao, *Anal. Chem.*, 2007, **79**, 6559.
- 15 S. Y. Zhu, L. He, F. Zhang, M. Y. Li, S. L. Jiao, Y. Li, M. Y. Chen, X. E. Zhao and H. Wang, *Talanta*, 2016, **161**, 169.
- 16 S. S. Ma, Y. X. Qi, X. Q. Jiang, J. Q. Chen, Q. Y. Zhou, G. Y. Shi and M. Zhang, *Anal. Chem.*, 2016, **88**, 111647.
- 17 X. E. Zhao, C. H. Lei, Y. Gao, H. Gao, S. Y. Zhu, X. Yang, J. M. You and H. Wang, *Sens. Actuators B: Chem.*, 2017, **253**, 239.
- 18 N. Li, Y. Li, Y. Han, W. Pan, T. Zhang and B. Tang, *Anal. Chem.*, 2014, **86**, 3924.
- 19 L. B. Li, C. Wang, J. X. Luo, Q. W. Guo, K. Y. Liu, K. Liu, K. Liu, W. J. Zhao and Y. Q. Lin, *Talanta*, 2015, **144**, 1301.
- 20 L. B. Li, C. Wang, K. Y. Liu, Y. H. Wang, K. Liu and Y. Q. Lin, *Anal. Chem.*, 2015, **87**, 3404.
- 21 X. Yang and E. K. Wang, *Anal. Chem.*, 2011, **83**, 5005.
- 22 H. C. Dai, P. J. Ni, Y. J. Sun, J. T. Hu, S. Jiang, Y. L. Wang and Z. Li, *Analyst*, 2015, **140**, 3616.
- 23 F. P. Shi, Y. Zhang, W. D. Na, X. Y. Zhang, Y. Li and X. G. Su, *J. Mater. Chem. B*, 2016, **4**, 3278.
- 24 Y. R. He, X. E. Zhao, S. Y. Zhu, N. Wei, J. Sun, Y. B. Zhou, S. Liu, Z. Q. Liu, G. Chen, Y. R. Suo and J. M. You, *J. Chromatogr. A*, 2016, **1458**, 70.
- 25 X. E. Zhao, Y. R. He, P. Yan, N. Wei, R. J. Wang, J. Su, L. F. Zheng, S. Y. Zhu and J. M. You, *RSC Adv.*, 2016, **6**, 108635.
- 26 S. S. Ma, Q. Y. Zhou, F. Y. Mu, Z. H. Chen, X. Y. Ding, M. Zhang and G. Y. Shi, *Analyst*, 2017, **142**, 3341.
- 27 J. Sun, B. Wang, X. Zhao, Z. J. Li and X. R. Yang, *Anal. Chem.*, 2016, **88**, 1355.
- 28 R. Li, C. H. Lei, X. E. Zhao, Y. Gao, H. Gao, S. Y. Zhu and H. Wang, *Spectrochim. Acta A*, 2018, **188**, 20.
- 29 S. P. Wu and S. Y. Meng, *Mater. Chem. Phys.*, 2005, **89**, 423.
- 30 X. Wang, P. Wu, X. Hou and Y. Lv, *Analyst*, 2013, **138**, 229.
- 31 X. J. Gong, Y. Liu, Z. H. Yang, S. M. Shuang and Z. Y. Zhang, *Anal. Chim. Acta*, 2017, **968**, 85.
- 32 M. C. Rong, L. P. Lin, X. H. Song, Y. R. Wang, Y. X. Zhong, J. W. Yan, Y. F. Feng, X. Y. Zeng and X. Chen, *Biosensor. Bioelectron.*, 2015, **68**, 210.
- 33 H. B. Rao, H. W. Ge, Z. W. Lu, W. Liu, Z. Q. Chen, Z. Y. Zhang, X. X. Wang, P. Zou, Y. Y. Yang, H. He and X. Y. Zeng, *Microchim. Acta*, 2016, **183**, 1651.
- 34 L. B. Li, C. Wang, K. Y. Liu, Y. H. Wang, K. Liu and Y. Q. Lin, *Anal. Chem.*, 2015, **87**, 3404.
- 35 M. Ganiga and J. Cyriac, *Anal. Bioanal. Chem.*, 2016, **408**, 3699.
- 36 Y. Cen, J. Tang, X. J. Kong, S. Wu, J. Yuan, R. Q. Yu and X. Chu, *Nanoscale*, 2015, **7**, 13951.
- 37 R. Liu, D. Wu, S. Liu, K. Koynov, W. Knoll and Q. Li, *Angew. Chem. Int. Ed.*, 2009, **48**, 4598.

Graphical Abstract

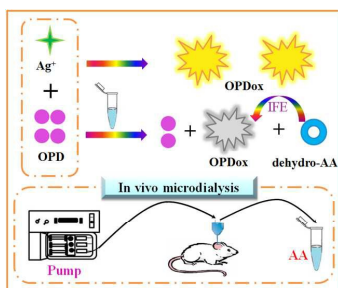A simple and label-free fluorescence detection of ascorbic acid in rat brain microdialysates in the presence of catecholaminesShuyun Zhu^{a,b*} †, Cuihua Lei^{a†}, Yue Gao^a, Jing Sun^b, Hongwei Peng^c, Han Gao^a, RuixueZhang^a, Rui Wang^a, Xian-En Zhao^{a,b*}, Hua Wang^{a*}

A facile and ultrasensitive sensor was constructed successfully for AA sensing based on the synergistic effect of reducing capability of AA and IFE.