


NAME NSK-1
EXPNO 138
PROCNO 1
Date_ 20180521
Time 16.54
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 0
SWH 10330.578 Hz
FIDRES 0.157632 Hz
AQ 3.1719923 sec
RG 203
DW 48.400 usec
DE 6.50 usec
TE 303.3 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 1H
P1 13.32 usec
PL1 2.00 dB
PL1W 17.43382454 W
SFO1 500.1330886 MHz
SI 32768
SF 500.1299943 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

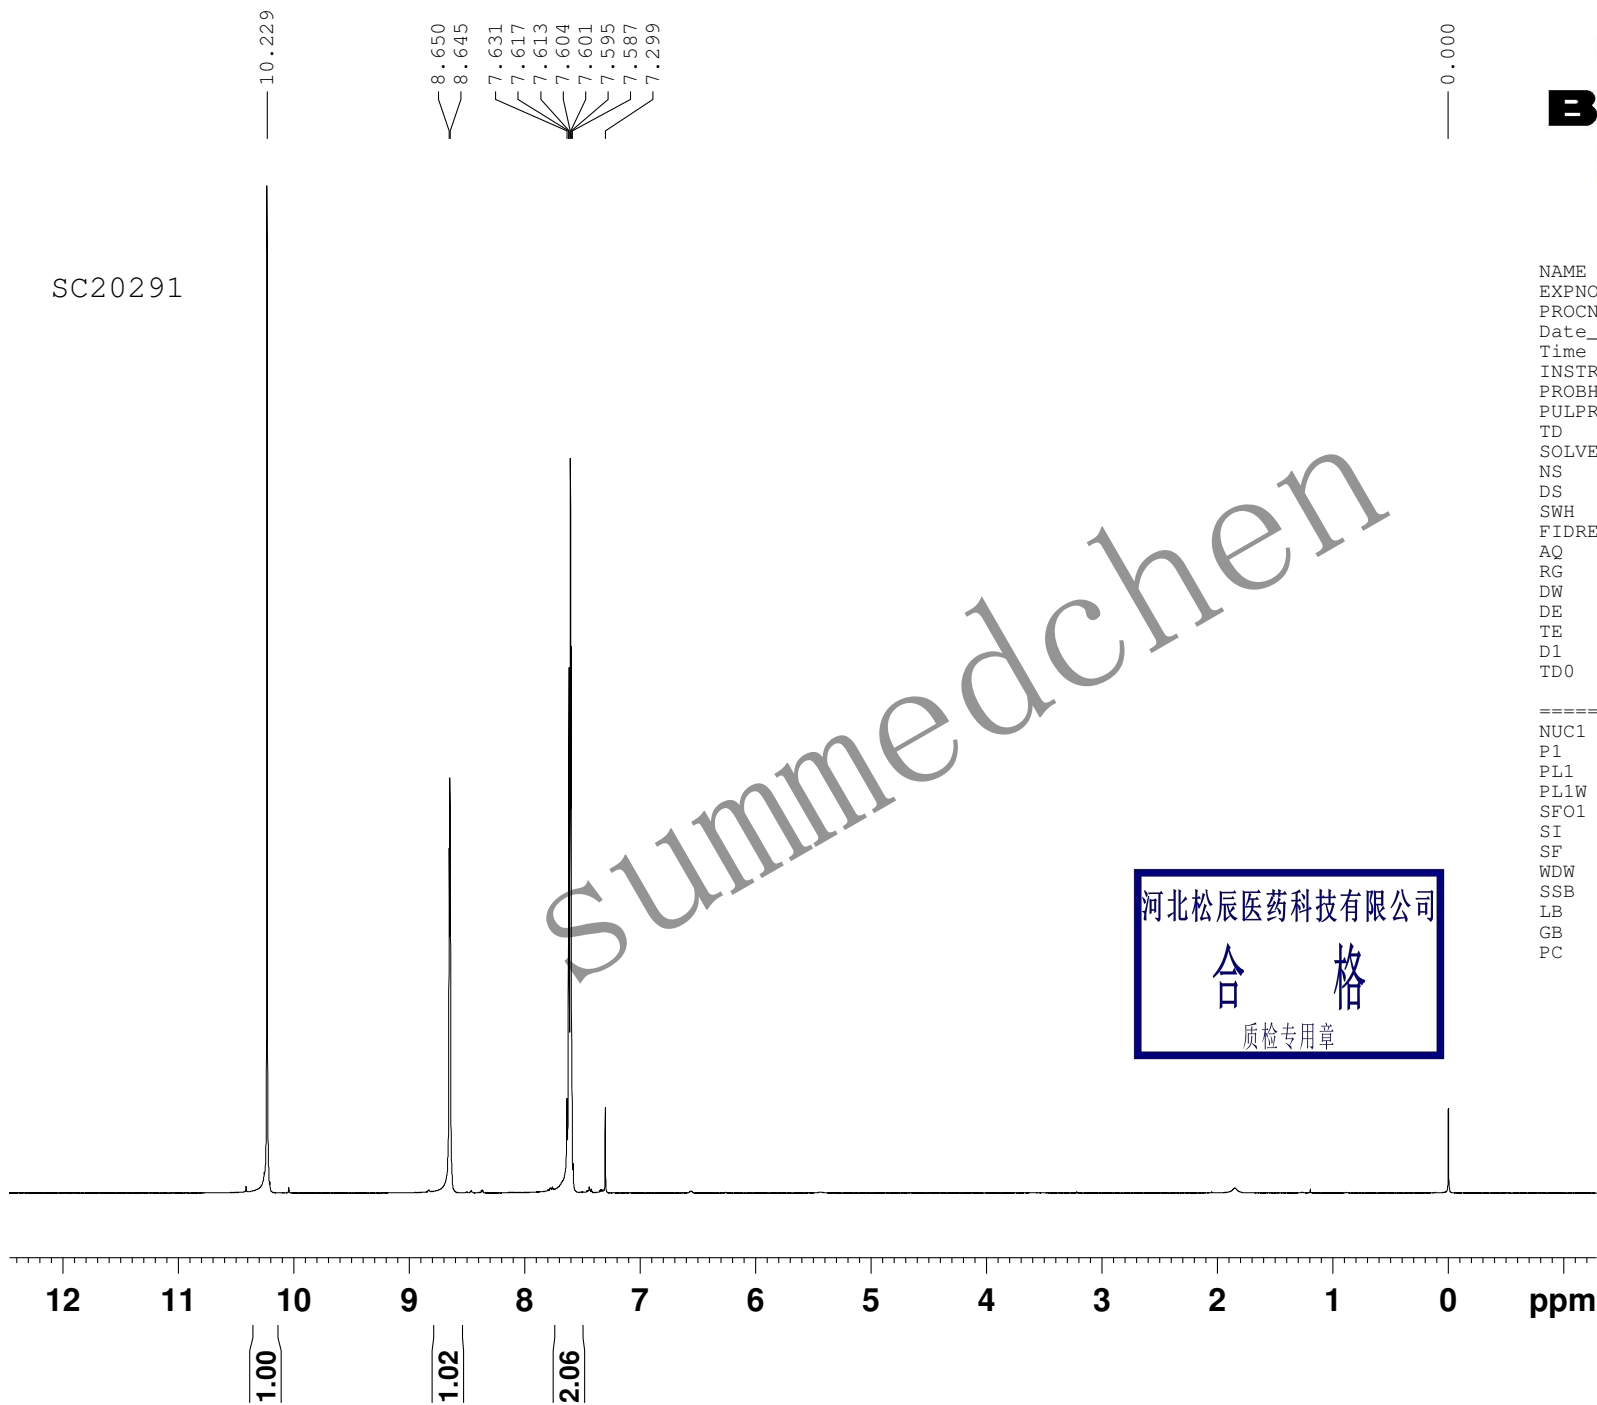

Summedchen

河北松辰医药科技有限公司
合格
质检专用章