




Data file: E:\DATA\180724\800071_18060014Final.D
Sample name: 800071_18060014Final
Description: Mobile phase: Buffer A: 0.1%TFA in H2O
Buffer B: 0.1%TFA in (40%ACN+60%H2O)
Gradient 10-35% in 20min, Flow rate: 1.0ml/min
Column: Unitary C18, 4.6*150mm, 5um 100A (A-001)
Instrument: Agilent HPLC 1100
Instrument: QC Location: 1
Injection date: 2018/7/24 8:58:52 Injection: 1 of 1
Last changed: 2018/7/24 9:26:03 Injection volume: 15.000
Acq. operator: QC_1

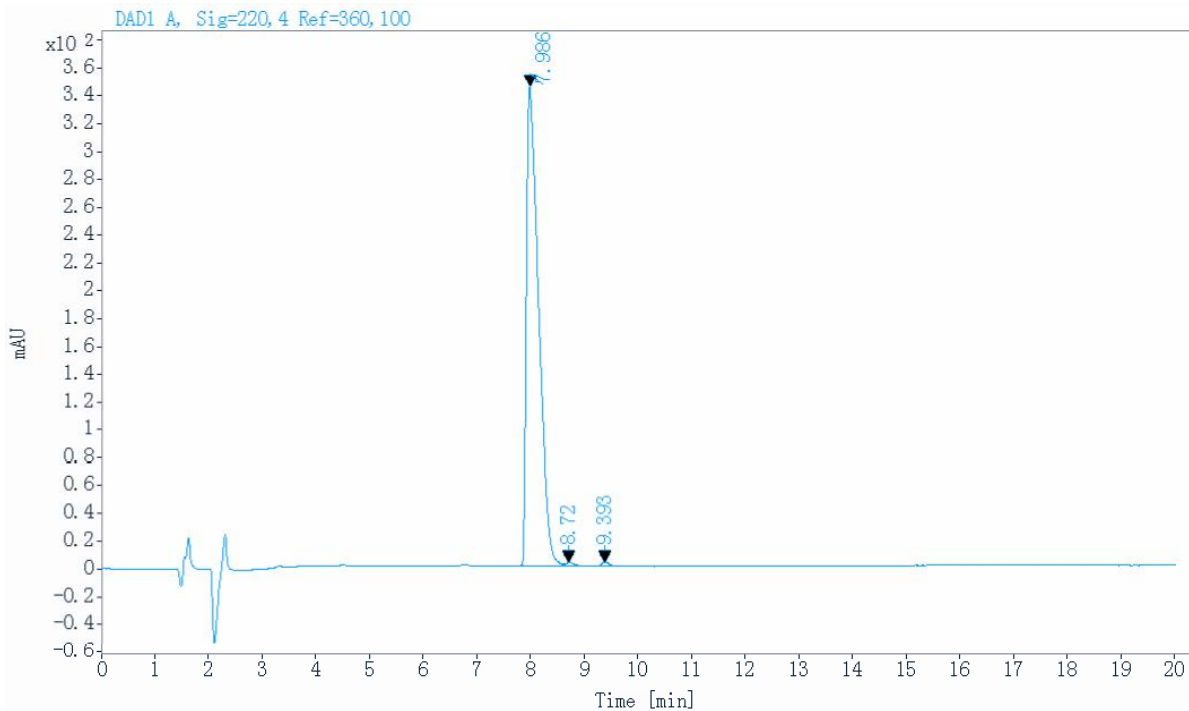

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area% Name
7.986	BV R	0.2429	5408.1162	344.8954	98.8544
8.720	VB E	0.2007	29.7498	2.1601	0.5438
9.393	BV R	0.1662	32.9225	3.0440	0.6018
Sum			5470.7885		