




Current Data Parameters
NAME RFS-STZF-H1-MEOD-20180724
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20180724
Time 14.39
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT MeOD
NS 16
DS 2
SWH 8223.685 Hz
FIDRES 0.125483 Hz
AQ 3.9846387 sec
RG 197.41
DW 60.800 usec
DE 8.00 usec
TE 297.8 K
D1 1.00000000 sec
TD0 1

==== CHANNEL f1 =====
NUC1 1H
P1 13.22 usec
PLW1 15.84899998 W
SFO1 400.1632013 MHz

F2 - Processing parameters
SI 65536
SF 400.1600000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

4.876
3.499
3.335
3.331
3.327
3.322
3.318
3.150
2.438
2.420
2.400
1.481
1.463
1.446
1.328
1.304
0.932
0.916
0.898

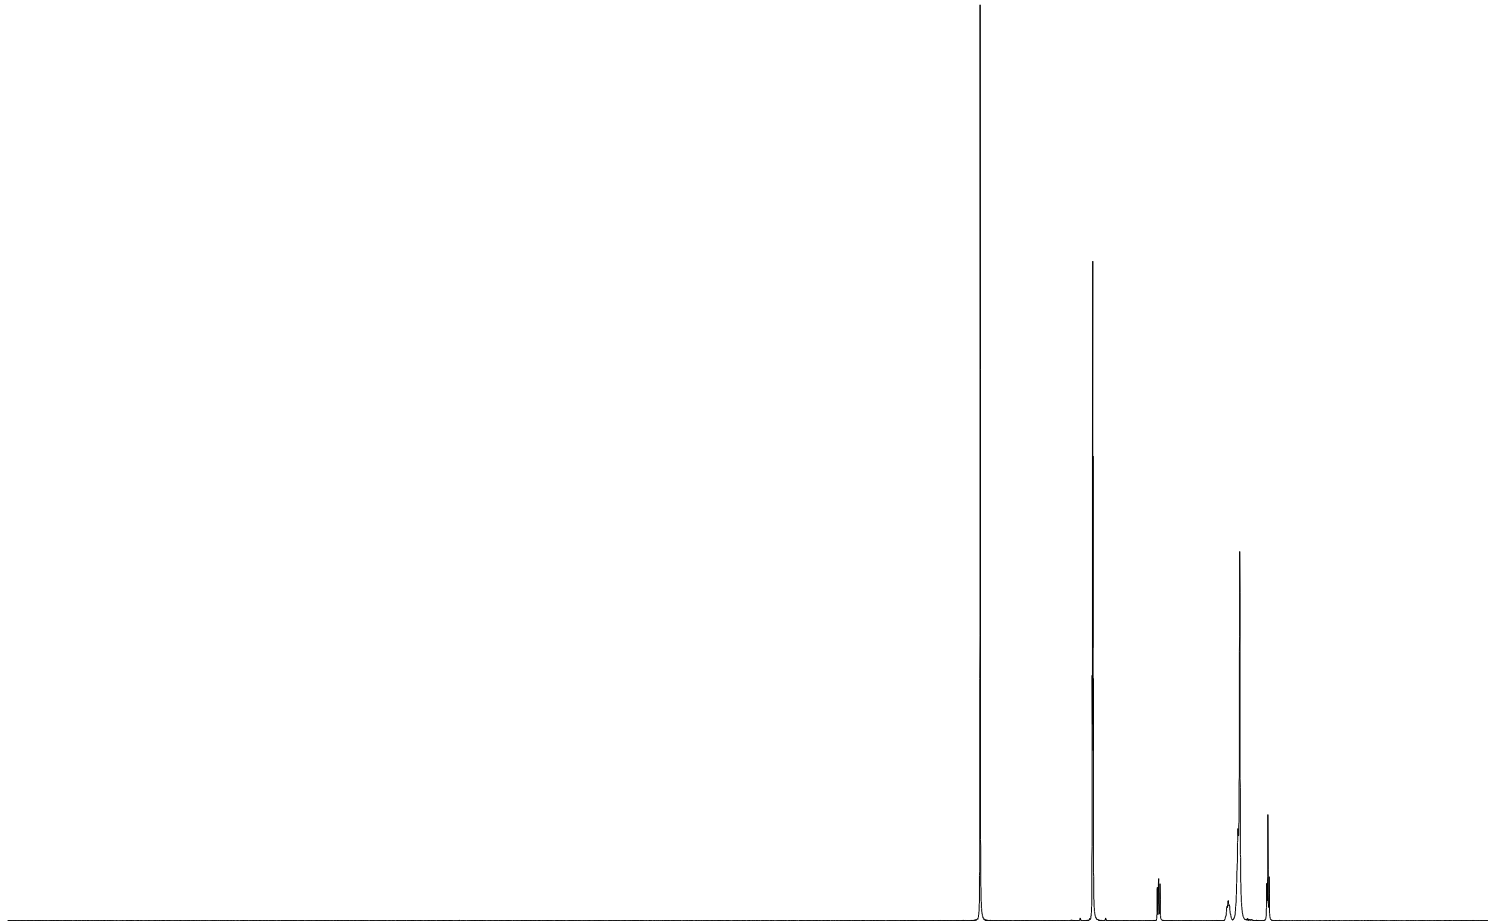

18 17 16 15 14 13 12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

2.0000
2.0573
5.1998
11.2292
3.0342