

Synthesis of silver nanoparticles-decorated FePO₄ nanosphere at a gas-liquid interface for the electrochemical detection of Hydrogen peroxide

DEJIANG RAO, JIAN ZHANG and JIANBIN ZHENG*

Institute of Analytical Science, Shaanxi Provincial Key Laboratory of Electroanalytical Chemistry,
Northwest University, Xi'an, Shaanxi 710069, China
e-mail: zhengjb@nwu.edu.cn

MS received 12 October 2015; revised 21 January 2016; accepted 19 February 2016

Abstract. Silver nanoparticles were prepared by chemical reduction of acetaldehyde gas in the absence of protective gas, and Ag/FePO₄ nanocomposites were synthesised by modified silver mirror reaction at a gas-liquid interface. A hydrogen peroxide (H₂O₂) electrochemical sensor was constructed through immobilizing Ag/FePO₄ nanocomposites on gold (Au) electrode. The morphology and composition of the nanocomposites were characterized by transmission electron microscopy (TEM) and energy-dispersive X-ray spectroscopy (EDS). The electrochemical investigations of the sensor indicated that it exhibited excellent analytical performance with a wide linear range from 3.0×10^{-5} to 1.1×10^{-2} mol·L⁻¹ and a low detection limit of 4.7 μmol·L⁻¹ at a signal-to-noise ratio of 3. Meanwhile, it also showed acceptable reproducibility and anti-interference ability. This study may provide a new method for the synthesis of highly dispersed metal nanoparticles which might be used in other related fields.

Keywords. Electrochemical sensor; gas-liquid interface; FePO₄; hydrogen peroxide; silver.

1. Introduction

Hydrogen peroxide (H₂O₂) plays vital roles in industry, biomedicine, pharmaceutical chemistry and many other fields.¹⁻³ Therefore, it is of great importance to develop an efficient method for selective and sensitive determination of H₂O₂. Many methods have been reported for detecting H₂O₂, such as titrimetry,⁴ fluorometry,⁵ chromatography,⁶ spectrophotometry,⁷ chemiluminescence⁸ and electrochemistry.⁹ Among these methods, the electrochemical detection methods have attracted more and more attention because of low cost, simplicity and high efficiency.¹⁰⁻¹² The electrochemical detection of H₂O₂ could be classified into two main categories: enzymatic detection and non-enzymatic detection. However, enzyme-based sensors suffer from the expensive enzyme material, poor stability and complex fabrication procedure for sensor.^{13,14} Thus, many people are committed to the study of non-enzymatic sensors. Moreover, with the emergence and development of nanotechnology, nanoparticles (NPs) play an important role in the non-enzymatic electrochemical sensors due to their good catalytic performance and biocompatibility.^{15,16} Especially, metal nanoparticles

with good catalytic properties and conductivity can be modified on the electrode. Among these nanoparticles, NPs of Pd,¹⁷ Cu,¹⁸ Au¹⁹ and Ag²⁰ have been used to construct electrochemical sensors for detecting H₂O₂.

Comparing with other metal nanoparticles, excellent catalytic properties of Ag NPs are getting greater attention of the researchers. Ag NPs have attracted much interest in the sensor applications due to their low cost, high surface-to-volume ratio and excellent conductivity.^{21,22} In addition, in our group, the dispersed AgNPs were synthesized by using methyl aldehyde as reducing agent at a gas-liquid interface, which could slow down the rate of reduction reaction, and thus the aggregation of AgNPs was avoided.²³

In recent years, phosphate nanomaterials have been reported, such as LiFePO₄,²⁴ AlPO₄,²⁵ and FePO₄.²⁶ Among them, FePO₄ is a particularly promising material because of good electrochemical activity and has aroused wide attention.^{27,28} Besides, FePO₄ nanosphere has many advantages, including environment-friendliness, low-cost, large surface area, good electron transfer capability and good thermal stability.²⁹⁻³¹ It has been reported that the amorphous FePO₄ nanosphere can be a catalyst supporter for loading Au NPs, and the obtained Au/FePO₄ catalyst can catalyze oxidation of

*For correspondence

CO.³² Therefore, FePO₄ nanosphere could also be used as a catalyst support with a great potential. The high surface-to-volume ratio and negative surface charge of FePO₄ nanosphere could provide a large surface to load more Ag NPs, and thereby improve the catalytic performance toward the reduction of H₂O₂. To the best of our knowledge, Ag NPs decorated FePO₄ nanosphere has never been reported so far. Besides, the synthetic method of FePO₄ nanosphere is much simpler than other catalyst supports such as graphene.³³

In this study, Ag/FePO₄ nanocomposites were prepared at a gas-liquid interface. Based on this, we developed a new type of non-enzymatic sensor for electrochemical detection of H₂O₂. This paper may provide a good catalyst support and a simple method for the development of H₂O₂ electrochemical sensors.

2. Experimental

2.1 Materials

Hydrogen peroxide (30%, v/v aqueous solution), acetaldehyde (C₂H₄O, 40%) and ammonium ferrous sulfate ((NH₄)₂Fe(SO₄)₂·6H₂O) were purchased from Tianjin Tianli Chemistry Reagent Co., Ltd (Tianjin, China); Chitosan (CS, MW 5–6 × 10⁵, >90% deacetylation) was purchased from Shanghai Yuanju Biotechnology Co, Ltd (Shanghai, China); 0.1 M phosphate buffered saline (PBS, pH 7.2) as the supporting electrolyte in electrochemical experiments. In addition, other reagents and chemicals were analytical reagent grade. Doubly distilled water was used in all the experiments.

2.2 Apparatus and Electrochemical Measurements

The transmission electron microscopic (TEM) measurements were executed with Tecnai G² F20 S-TWIN (FEI, USA). The energy-dispersive X-ray spectroscopy (EDS) was performed during the scanning electron microscopic JSM-6700F (JEOL, Japan) measurements.

Electrochemical measurements were executed with a classical three-electrode electroanalysis system of CHI 660 electrochemical workstation (Shanghai CH Instrument Co. Ltd., China). The bare Au electrodes (diameter: 2.0 mm), FePO₄ modified Au electrode and Ag/FePO₄ modified Au electrode were used as working electrodes in respective experiments. The saturated calomel electrode (SCE) and platinum wire electrode were used as the reference electrode and counter electrode, respectively. The whole experiment was conducted at room temperature (25 ± 2°C).


2.3 Fabrication of the Sensor

2.3a Synthesis of FePO₄ nanospheres: (NH₄)₂Fe(SO₄)₂·6H₂O (0.4 g), urea (1.0 g) H₃PO₄ (14 μL) and sodium dodecylsulfate (SDS, 0.1 g) were dissolved in 20 mL doubly distilled water. The mixture was stirred vigorously for about ten minutes, and then decanted into a 25 mL-Teflon-lined autoclave, heated and kept at 80°C for 12 h. The autoclave was naturally cooled to room temperature after completion of the reaction. The final sediment was collected by centrifugation at 7000 rpm for 8 min, washed twice with doubly distilled water and then dried at 6°C for 12 h.

2.3b Synthesis of Ag/FePO₄: 10 mL of AgNO₃ (10 mM) was added to a 25 mL beaker containing 10 mL of doubly distilled water. Then, 200 μL of NaOH (1 mol L⁻¹) solution was added to this beaker under stirring condition until a fine brown precipitate of Ag₂O was formed. The brown precipitate of Ag₂O gradually disappeared until clarification when 25% NH₃·H₂O (300 μL) was added drop by drop under stable stirring condition. Ag[(NH₃)₂]⁺ solution (4.88 mM) was prepared and left for future use.

FePO₄ powder (15 mg) was completely dispersed to 45 mL of ethanol-water (1:1, v/v) solution by ultrasound for 30 min, and then ultrasonically mixed with 5 mL of above as-prepared Ag[(NH₃)₂]⁺ solution. After a while, the mixture and another beaker which with 10 mL of CH₃CHO solution were placed in a sealed beaker. This modified silver mirror reaction was performed for 1 h under stable stirring at room temperature. The composite products was collected by centrifugation at 7000 rpm for 8 min, washed thrice with doubly distilled water, and then dried at 5°C for 10 h.

2.3c Modification of electrode: The Au electrode was prepared by a simple method. Before use, the Au electrode was polished with 1.0 and 0.3 μm alumina powder to obtain a mirror-like surface. Then washed with doubly distilled water, completely cleaned in ethanol solution and doubly distilled water in proper order under ultrasonic condition. The Au electrode was dried in a stream of nitrogen. 1 mg of Ag/FePO₄ nanocomposite was dispersed in 1 mL of chitosan (wt%, 0.5%) solution under ultrasonic condition for 30 min. The obtained suspension (5 μL) was dropped to the surface of Au electrode and dried in air at room temperature. The modified electrode can be labeled as Ag/FePO₄/Au electrode. The process of the synthesis of the material and the modification of the electrode are shown in scheme 1.



Scheme 1. Schematic illustration for the synthesis of Ag/FePO₄ nanocomposite and modification of the Au electrode.

3. Results and Discussion

3.1 Characterization of Ag/FePO₄ Nanocomposites

The transmission electron microscopic (TEM) measurements are an efficient tool to characterize the morphology of nanocomposites. The morphology of FePO₄ (A, B) and Ag/FePO₄ (C, D) nanocomposites are shown in figure 1. From figure 1A and B we can know that the FePO₄ composite was more likely a spherical nanomaterial with an average diameter of 650 ± 50 nm. Compared with figure 1D, it is clearly seen that FePO₄ nanospheres were successfully decorated with well-dispersed Ag nanoparticles according to the synthesis method. The average diameter of Ag NPs is ranging from 8 to 10 nm. Moreover, a large amount of Ag NPs with small spherical particles were observed uniformly on the surface of the FePO₄ nanosphere. Furthermore, the EDS analysis had also been used to characterize the elements in Ag/FePO₄ nanocomposites. The EDS spectrum is shown in figure S1 in Supplementary Information.

3.2 Electrochemical behavior of Ag/FePO₄

Electrochemical impedance spectroscopy (EIS) is a powerful tool to investigate the interfacial properties of chemically modified electrodes. Generally, the semicircle diameter of the nyquist plot represents the electron transfer resistance (R_{ct}).³⁴ The suitable equivalent circuit obtained by CHI 660 software is shown in figure 2.

Here, R_s is the ohmic resistance of the electrolyte solution; Cdl indicates an ideal capacitor; Q is used to represent a constant phase element which is an accumulation of all capacitive effects in the measurement; R_{et} is the interfacial electron-transfer resistance and W is a Warburg impedance which models the diffusion of ions from the bulk electrolyte to the electrode. As shown in figure 2, the diameter of semicircle of the Ag/FePO₄/Au electrode (curve a) is smaller than those of the bare Au electrode (curve b) and FePO₄/Au electrode (curve c). Moreover, the semicircle diameter has increased from 50Ω to 300Ω when the FePO₄ is fixed to the surface of Au electrode. However, the R_{et} decreased extremely after addition of the Ag NPs to the surface of FePO₄ composite. It should be noted that the curve for the Ag/FePO₄/Au electrode looks approximately like a straight line in that frequency range, indicating that the R_{et} of the Ag/FePO₄ is pretty small. Therefore, the Ag/FePO₄ could efficiently enhance the electron transfer efficiency.

Figure 3 shows the electrochemical responses of the bare Au electrode, FePO₄ modified Au electrode and Ag/FePO₄ modified Au electrode as working electrode, respectively. The red arrow indicates the direction of sweep (as in other CVs). From the figure 3, we can know that the bare Au electrode (curve b), FePO₄ modified Au electrode (curve c) and Ag/FePO₄ modified Au electrode (curve a) show almost no electrochemical response in the absence of H₂O₂. However, the electrochemical responses have been changed




Figure 1. TEM images of FePO₄ (A, B), and Ag/FePO₄ (C, D).




Figure 2. Nyquist plots of (a) Ag/FePO₄/Au electrode, (b) bare Au electrode and (c) FePO₄/Au electrode in KCl solution (0.10 M) containing 5.0 mM [Fe(CN)₆]^{4-/3-} at open-circuit potential conditions. Frequency range: 0.01 Hz to 10 kHz; AC amplitude: 5.0 mV. Inset: Equivalent electrical circuit obtained by CHI 660 software.




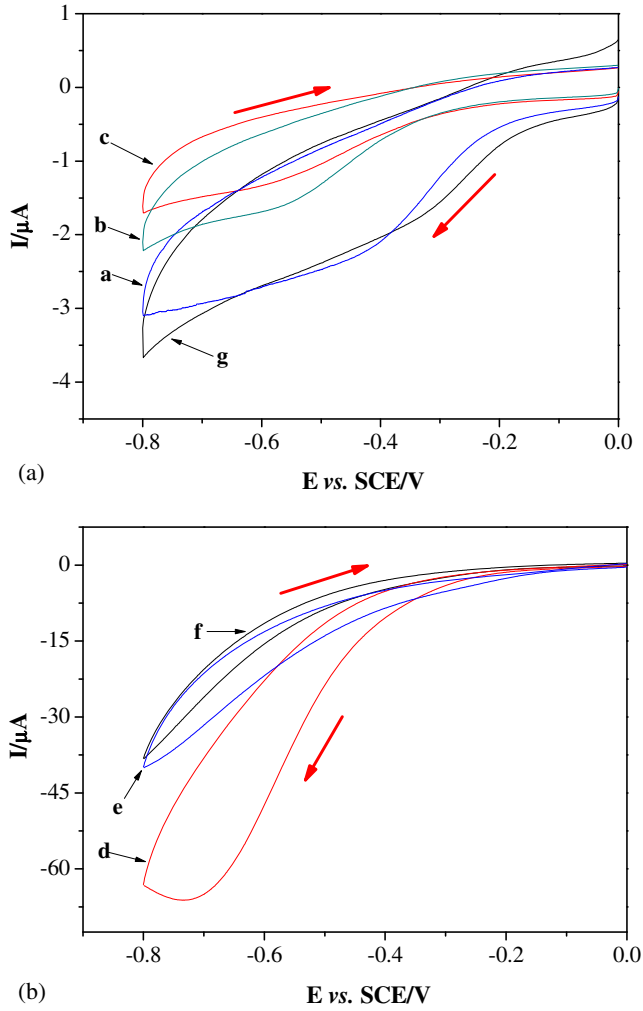




Figure 3. CV curves (b, e) of bare Au electrode and (c, f) FePO₄ modified Au electrode and (a, d) Ag/FePO₄ modified Au electrode in N₂-saturated 0.1 M PBS (pH 7.2) in the absence (b, c and a) and presence (e, f and d) of 5 mM H₂O₂ at a scan rate of 0.1 V/s. (curve g) Ag/FePO₄/Au electrode in O₂-saturated 0.1 mol·L⁻¹ PBS (pH 7.2) in the absence of H₂O₂.

significantly when 5 mM H₂O₂ was added (figure 3B). Comparing with Ag/FePO₄ modified Au electrode (curve d), the bare Au electrode (curve e) and FePO₄ modified Au electrode (curve f) exhibited low electrochemical responses. The CV curves of Ag/FePO₄/Au electrode (curve g) in O₂-saturated 0.1 M PBS (pH 7.2) in the absence of H₂O₂ are shown in figure 3A. The reduction current of oxygen was small enough to be negligible. It shows that oxygen had a negligible effect in the electrochemical experiments. The Ag/FePO₄ modified Au electrode showed an apparent catalytic current peak of approximately -65 μA at nearly -0.72 V. Thus, the Ag/FePO₄ nanocomposites show good catalytic performance towards the electro-reduction of H₂O₂.


The mechanism of H₂O₂ electro-reduction can be expressed as follows:³⁵




When the surface of the electrode is modified by the Ag NPs, the cathodic reaction is the reduction of H₂O₂ as the first electron transfer reaction and the anodic reaction is the dissolution of Ag NPs. Actually, the Ag NPs disproportionate the balance of the reaction and speed up the reaction rate in the buffer solution, and the reaction becomes more irreversible.³⁵



However, the presence of oxygen in the above action could become the detection signal on electrode. The electroreduction of O₂ on electrode occurs by the mechanism shown below.³⁶



Then,



Because of the excellent catalytic properties of Ag NPs for H₂O₂, the response signal of H₂O₂ was detected after Ag NPs were fixed on the surface of FePO₄.

The amount of as-prepared [Ag(NH₃)₂]⁺ solution is critical to electrochemical experiments because Ag NPs could enhance the electron transfer efficiency for the determination of H₂O₂.²³ The different amounts of as-prepared [Ag(NH₃)₂]⁺ solution can be used to synthesize Ag/FePO₄ nanocomposites decorated with different amounts of Ag NPs. Therefore, the Ag/FePO₄ nanocomposites with different amounts of Ag NPs were prepared to construct the modified electrode to detect H₂O₂ by CVs. The experimental results are shown in figure 4. As seen in figure 4, the peak current increased at the beginning and then decreased with the raise of [Ag(NH₃)₂]⁺ solution and the maximum peak current was observed with 6 mL as-prepared [Ag(NH₃)₂]⁺ solution. However, more Ag NPs were easily aggregated and the catalytic properties were then reduced. Therefore, we chose 5.0 mL of as-prepared [Ag(NH₃)₂]⁺ solution as appropriate.

The reduction peak current increased with the increasing concentration of H₂O₂ from 0.5 to 5.0 mM




Figure 4. The current response (peak current) values obtained by Ag/FePO₄/Au electrode in N₂-saturated 0.1 M PBS (pH 7.2) containing 5 mM H₂O₂ at a scan rate of 0.1 V s⁻¹ with different amounts of 4.88 mM as-prepared [Ag(NH₃)₂]⁺ (3, 4, 5, 6, 7 and 8 mL).




Figure 5. CV curves of Ag/FePO₄ modified Au electrode in the presence of different H₂O₂ concentrations (from a to j: 0.5, 1, 1.5, 2, 2.5, 3, 3.5, 4, 4.5 and 5.0 mM) in N₂-saturated 0.1 M PBS (pH 7.2) at a scan rate of 0.1 V s⁻¹. Inset: Linear fitting of the reduction peak current with H₂O₂ concentration.

on the Ag/FePO₄ modified Au electrode as shown in figure 5. Figure 5 inset shows that there is a good linear relationship ($R = 0.9986$) between reduction peak current and concentration of H₂O₂. These results strongly demonstrate that the Ag/FePO₄ nanocomposites had remarkable electrocatalytic performance towards H₂O₂.

The reduction current at different scan rates with 4.0 mM H₂O₂ is shown in figure 6. The reduction peak current changed linearly with the square root of the scan rate when the scan rate gradually increased from 0.02 to 0.14 V s⁻¹. Therefore, the electrochemical




Figure 6. CV curves of the Ag/FePO₄ modified Au electrode in N₂-saturated 0.1 M PBS (pH 7.2) containing 4.0 mM H₂O₂ at different scan rates (from a to g: 0.02, 0.04, 0.06, 0.08, 0.10, 0.12, 0.14 V s⁻¹). Inset: Linear fitting of reduction peak current versus $v^{1/2}$.

process of H₂O₂ reduction on the Ag/FePO₄ modified Au electrode is diffusion-controlled.

Figure 7A shows the amperometric current–time curve of the Ag/FePO₄ modified Au electrode in N₂-saturated 0.1 M PBS (pH 7.2) under stirring condition. The calibration curve for the Ag/FePO₄ modified Au electrode is shown in figure 7B. It can be observed that the Ag/FePO₄ modified Au electrode exhibits quick response within 4 s. The linear regression equation is $I_p (\mu A) = -2.6 C (mM) - 1.24$ with a correlation coefficient of 0.9995. Moreover, the Ag/FePO₄ modified Au electrode has linear amperometric response to concentration of H₂O₂ in the range of $3 \times 10^{-5} - 1.1 \times 10^{-2}$ M is shown in figure 7B. The sensitivity and detection limit were calculated to be 82.8 $\mu A cm^2 mM^{-1}$, 4.7 μM (Signal-to-noise ratio: 3), respectively. The comparison of the performance of our sensor with other non-enzymatic H₂O₂ sensors are listed in table 1. It is noticeable that our sensor had higher sensitivity than other reported sensors. In addition, our sensor has an acceptable linear range and detection limit. The good performance may be because excellent electrocatalytic properties of AgNPs for electro-reduction of H₂O₂.

3.3 Interference Study

The amperometric response of the Ag/FePO₄ modified Au electrode upon the injection of H₂O₂ (0.5 mM) and other electroactive species (0.5 mM) in N₂-saturated 0.1 M PBS (pH 7.2) with stirring condition at -0.45 V are shown in figure 8A. The addition of 0.5 mM H₂O₂ exhibits an obvious amperometric response, while the

amperometric current was not changed obviously when glucose, ethanol, ascorbic acid (AA) and uric acid (UA) were added. The amperometric response of the Ag/FePO₄ modified Au electrode in O₂-saturated (curve a) and N₂-saturated (curve b) 0.1 M PBS are shown in figure 8B. From the figure 8B, we can clearly see the

stability of the current responses and a good signal-to-noise ratio in N₂-saturated 0.1 M PBS at −0.45 V (curve b). The background noise increased because of the electro-reduction of O₂ when it was detected in O₂-saturated 0.1 M PBS (curve a). But the response current

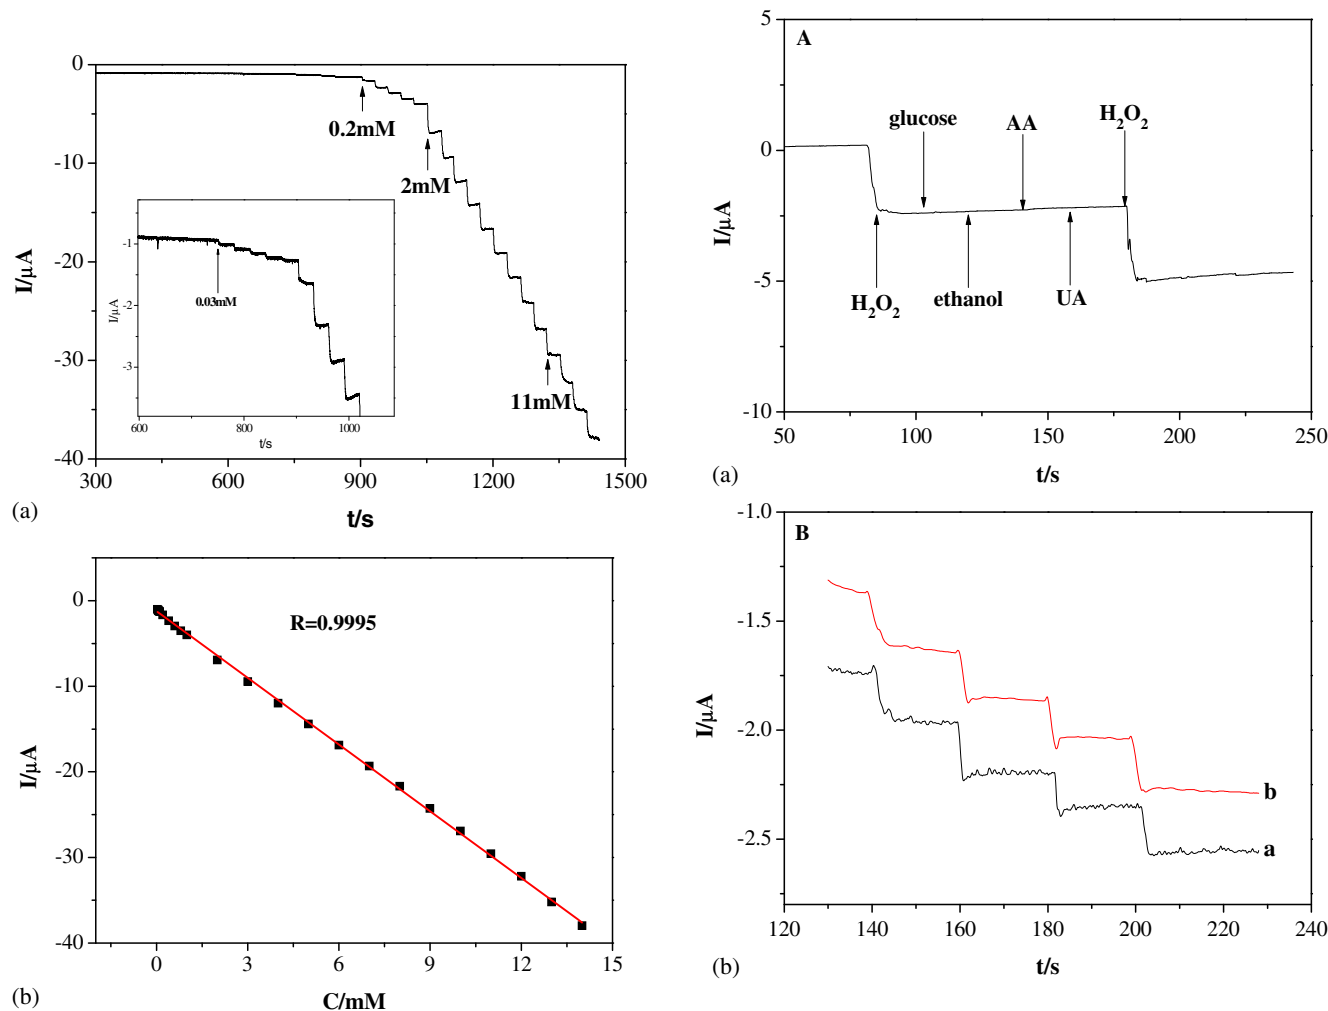


Figure 7. (A) Amperometric response of the Ag/FePO₄ modified Au electrode upon successive injection of H₂O₂ in N₂-saturated 0.1 M PBS (pH 7.2) under stirring condition. Applied potential: −0.45 V. Inset: Amplification of the plot for low concentrations. (B) Calibration curve of current versus its concentration.

Figure 8. (A) Amperometric response of the Ag/FePO₄ modified Au electrode to successive addition of H₂O₂, glucose, ethanol, ascorbic acid (AA), and uric acid (UA) (0.5 mM, respectively) in N₂-saturated 0.1 M PBS (pH 7.2) under stirring condition. (B) Successive addition of H₂O₂ (0.15 mM) in (a) O₂-saturated and (b) N₂-saturated 0.1 M PBS (pH 7.2). Applied potential: −0.45 V.

Table 1. Comparison of analytical performance of our H₂O₂ sensor with other non-enzymatic H₂O₂ sensors.

Sensors	Applied potential (V)	Linear range (mM)	Sensitivity (μA mM ⁻¹ cm ⁻²)	Detection limit (μM)	References
Ag-PQ11/GCE	−0.30	0.1–180	—	33.9	37
Ag/MWCNT/Au electrode	−0.20	0.05–17	20	0.50	38
MnO ₂ /carbon fiber microelectrode	+0.58	0.012–0.26	10.6	5.4	39
Ag-CP/GCE	−0.30	0.7–70	—	0.9	40
Ag@TiO ₂ /GCE	−0.73	0.83–43.3	25.23	0.83	41
Ag/FePO ₄ /Au electrode	−0.45	0.03–11	82.8	4.7	This study

Table 2. H₂O₂ detection in detergent samples by the standard addition method.

Sample	H ₂ O ₂ added (mM)	H ₂ O ₂ found (mM) (n = 3) [*]	Recovery (%)
detergent sample	—	0.142 (±0.03)	—
Sample 1	0.1	0.240 (±0.05)	98.0
Sample 2	0.25	0.389 (±0.03)	98.8
Sample 3	1.5	1.651 (±0.02)	100.6

^{*}Average of three determinations (± relative standard deviation).

almost remained unchanged. So the Ag/FePO₄ modified Au electrode exhibited excellent performance of anti-interference to O₂. Hence we conclude that the H₂O₂ sensor has a favorable ability of anti-interference to other electroactive species and O₂.

3.4 Repeatability and stability study

The repeatability and stability of Ag/FePO₄ modified Au electrode is extremely important for the entire experiment. The amperometric current responses of five the Ag/FePO₄ modified Au electrodes at −0.45 V are compared. The relative standard deviation (RSD) was about 3%, so the modified electrode has good repeatability. The Ag/FePO₄ modified electrode remained at 90% of its initial current response after four weeks. To sum up, the Ag/FePO₄ modified electrode has acceptable reproducibility and stability.

3.5 Real sample analysis

The real sample analysis of our H₂O₂ sensor was tested for detecting a detergent by the standard addition method. Briefly, the detergent sample (1.0 mL) was added to 9.0 mL of 0.1 M PBS (pH 7.2) and recorded the amperometric responses of H₂O₂ reduction in N₂-saturated 0.1 PBS. The experimental results are listed in table 2. It is noticed that our H₂O₂ sensor could be used for the detection of H₂O₂ in the real samples.

4. Conclusions

In summary, the Ag/FePO₄ nanocomposites were synthesized by a modified silver mirror reaction at gas-liquid interface. Then the non-enzymatic H₂O₂ sensor was fabricated using this nanocomposites modifying the surface of the gold electrode. The non-enzymatic H₂O₂ electrochemical sensor presents excellent catalytic performance for the detection of H₂O₂ with a wide linear range and anti-interference ability. This study may be propitious to develop new methods for H₂O₂ electrochemical sensors.

Supplementary Information (SI)

The EDS spectrum of Ag/FePO₄ nanocomposites (figure S1) is given in the supporting information available at www.ias.ac.in/chemsci.

Acknowledgements

The authors gratefully acknowledge the financial support of this project by the National Science Fund of China (No. 21275116), Specialized Research Fund for the Doctoral Program of Higher Education (No. 20126101120023), the Natural Science Fund of Shaanxi Province in China (No. 2012JM2013, 2013KJXX-25), the Fund of Shaanxi Province Educational Committee of China (No. 12JK0576), the Scientific Research Foundation of Shaanxi Provincial Key Laboratory (2010JS088, 11JS080, 12JS087, 12JS088, 13JS097, 13JS098) and the Graduate Innovation Fund of Northwest University (No. YZZ12019).

References

1. Sanderson W R 2000 *Pure. Appl. Chem.* **72** 1289
2. Barnard J P and Stinson M W 1999 *Infect. Immun.* **67** 6558
3. Karthega M, Nagarajan S and Rajendran N 2010 *Electrochim. Acta* **55** 2201
4. Klassen N V, Marchington D and McGowan H C E 1994 *Anal. Chem.* **66** 2921
5. Gao Y, Wang G N, Huang H, Hu J J, Shah S M and Su X G 2011 *Talanta* **85** 1075
6. Steinberg S M 2013 *Environ. Monit. Assess.* **185** 3749
7. Hoshino M, Kamino S, Doi M, Takada S, Mitani S, Yanagihara R and Fujita Y 2014 *Spectrochim. Acta A* **117** 814
8. Shi W B, Zhang X D, He S H and Huang Y M 2011 *Chem. Commun.* **47** 10785
9. Liu M M, Liu R and Chen W 2013 *Biosens. Bioelectron.* **45** 206
10. Abdulrahman O 2013 *Nanoscale* **5** 8921
11. Zhang J and Zheng J B 2015 *Anal. Methods* **7** 1788
12. Mase K, Ohkubo K and Fukuzumi S 2013 *J. Am. Chem. Soc.* **135** 2800
13. Welch C M, Banks C E, Simm A O and Compton R G 2005 *Anal. Bioanal. Chem.* **382** 12

14. Long L H, Hoi A and Halliwell B 2010 *Arch. Biochem. Biophys.* **501** 162
15. Landon P, Collier P J, Papworth A J, Kiely C J and Hutchings G J 2002 *Chem. Commun.* **18** 2058
16. Zhang J D and Oyama M 2005 *J. Electroanal. Chem.* **577** 273
17. Jiang F X, Yue R R, Du Y K, Xu J K and Yang P 2013 *Biosens. Bioelectron.* **44** 127
18. Luo B B, Li X M, Yang J C, Li X L, Xue L P, Li X L, Gu J K, Wang M Z and Jiang L 2014 *Anal. Methods* **6** 1114
19. Jia F F, Zhong H, Zhu F X, Li X H, Wang Y Z, Cheng Z P, Zhang L L, Sheng Z H and Guo L P 2014 *Electroanal.* **26** 2244
20. Yadav D K, Gupta R, Ganesan V, Sonkar P K and Rastogi P K 2016 *J. Appl. Electrochem.* **46** 103
21. Michaels A M, Jiang J and Brus L 2000 *J. Phys. Chem. B* **104** 11965
22. Iga M, Seki A and Watanabe K 2004 *Sens. Actuators, B* **101** 368
23. Bai W S, Nie F, Zheng J B and Sheng Q L 2014 *ACS Appl. Mater. Inter.* **6** 5439
24. Huang H, Yin S C and Nazar L F 2001 *Electrochem. Solid-State Lett.* **4** A170
25. Lee J G, Kim B, Cho J, Kin Y W and Park B 2004 *J. Electrochem. Soc.* **151** A801
26. Prosini P P, Lisi M, Scaccia S, Carewska M, Cardellini F and Pasquali M 2002 *J. Electrochem. Soc.* **149** A297
27. Qing C B, Bai Y, Yang J M and Zhang W F 2011 *Electrochim. Acta* **56** 6612
28. Laffont L, Delacourt C, Gibot P, Wu M Y, Kooyman P, Masquelier C and Tarascon J M 2006 *Chem. Mater.* **18** 5520
29. Song Y N, Yang S F, Zavalij P Y and Whittingham M S 2002 *Mater. Res. Bull.* **37** 1249
30. Okada S, Yamamoto T, Okazaki Y, Yamaki J I, Tokunaga M and Nishida T 2005 *J. Power Sources* **146** 570
31. Shi Z C, Li Y X, Ye W L and Yang Y 2005 *Electrochem. Solid-State Lett.* **8** A396
32. Li M J, Wu Z L, Ma Z, Schwartz V, Mullins D R, Dai S and Overbury S H 2009 *J. Catal.* **266** 98
33. Yin Y J, Wu P, Zhang H and Cai C X 2012 *Electrochem. Commun.* **18** 1
34. Chen D, Wang G, Lu W, Zhang H and Li J H 2007 *Electrochem. Commun.* **9** 2151
35. Masataka H, Takuro K and Hideaki K 1986 *Electrochim. Acta* **31** 377
36. Xu J, Huang W H and McCreery R L 1996 *Electroanal. Chem.* **410** 235
37. Lu W B, Liao F, Luo Y L, Chang G H and Sun X P 2011 *Electrochim. Acta* **56** 2295
38. Zhao W, Wang H C, Qin X, Wang X S, Zhao Z X, Miao Z Y, Chen L L, Shan M M, Fang Y X and Chen Q 2009 *Talanta* **80** 1029
39. Hocevar S B, Ogorevc B, Schachl K and Kalcher K 2004 *Electroanalysis* **16** 1711
40. Luo Y L, Lu W B, Chang G H, Liao F and Sun X P 2011 *Electrochim. Acta* **56** 8371
41. Liu S, Tian J Q, Wang L, Li H Y, Zhang Y W and Sun X P 2010 *Macromolecules* **43** 10078