

A Turn-On Fluorescent Sensor for Detecting Nickel in Living Cells

Sheel C. Dodani, Qiwen He, and Christopher J. Chang*

Department of Chemistry and the Howard Hughes Medical Institute, University of California, Berkeley, California 94720

Received August 1, 2009; E-mail: chrischang@berkeley.edu


Nickel is an essential metal nutrient for supporting life, but loss of nickel homeostasis is harmful to prokaryotic and eukaryotic organisms alike.¹ Elegant studies continue to elucidate mechanisms for Ni²⁺ uptake, regulation, and efflux,^{2–10} as well as to define the redox and nonredox roles of nickel biochemistry in microbial and plant systems.^{11–17} However, the contributions of nickel homeostasis to mammalian health and disease remain largely unexplored.¹⁸ In this context, excess nickel accumulation can aberrantly affect respiratory and immune systems, but mechanisms of nickel imbalance are insufficiently understood.^{19,20}

To help elucidate the roles of nickel in living systems, we are developing Ni²⁺-selective fluorescent indicators as part of a larger program aimed at studying metals in biology by molecular imaging.^{21,22} Such chemical tools, in principle, can be used to monitor exchangeable nickel pools with spatial and temporal resolution and provide a complement to standard bulk techniques for measuring total nickel content such as atomic absorption or inductively coupled plasma mass spectrometry. A major chemical challenge to this end is designing systems with Ni²⁺-specific responses over other biologically relevant metal ions in water. Examples of Ni²⁺-responsive fluorescent probes remain rare; Ni²⁺-selective peptide,^{23,24} protein,²⁵ polymer,^{26,27} and small-molecule based sensors^{28–30} have been reported but have not been utilized for cellular imaging, whereas the commercial Zn²⁺ sensor Newport Green DCF also responds to Ni²⁺ and Ti³⁺ and has been used to detect their accumulation in cells.^{31–34} In this report, we present the synthesis and properties of Nickelsensor-1 (NS1, **5**), a new turn-on fluorescent sensor for the selective detection of Ni²⁺ in water and in biological samples. NS1 features visible wavelength spectral profiles and a ca. 25-fold fluorescence increase upon Ni²⁺ binding. Confocal microscopy experiments show that this indicator can reliably monitor changes in Ni²⁺ levels within living mammalian cells.

Our design for NS1 combines a BODIPY dye reporter with a mixed N/O/S receptor to satisfy the Ni²⁺ cation (Scheme 1). Addition of ditosylate **1** to Cs₂CO₃ and methyl thioglycolate affords diester **2** in 41% yield. Vilsmeier formylation of **2** using POCl₃/DMF followed by basic workup furnishes aldehyde **3** in 60% yield. BODIPY **4** is obtained in a one-pot, three-step procedure via condensation of **3** with 2,4-dimethylpyrrole, followed by DDQ oxidation and boron insertion with BF₃•OEt₂ (38% overall yield for three steps). Ester hydrolysis of **4** under basic conditions gives NS1 (**5**) in 71% yield.

Spectroscopic evaluation of NS1 was performed in 20 mM HEPES buffered to pH 7.1. The optical features of the probe are characteristic of the BODIPY platform. Apo NS1 displays one visible region absorption band centered at 495 nm ($\epsilon = 5.8 \times 10^3 \text{ M}^{-1} \text{ cm}^{-1}$) and an emission maximum at 507 nm ($\Phi = 0.002$). Addition of 50 equiv of Ni²⁺ triggers a ca. 25-fold fluorescence turn-on ($\Phi = 0.055$, Figure 1a) with no shifts in absorption ($\lambda_{\text{abs}} = 495 \text{ nm}$, $\epsilon = 5.5 \times 10^3 \text{ M}^{-1} \text{ cm}^{-1}$) or emission maxima ($\lambda_{\text{em}} =$

Scheme 1. Synthesis of Nickelsensor-1 (NS1)

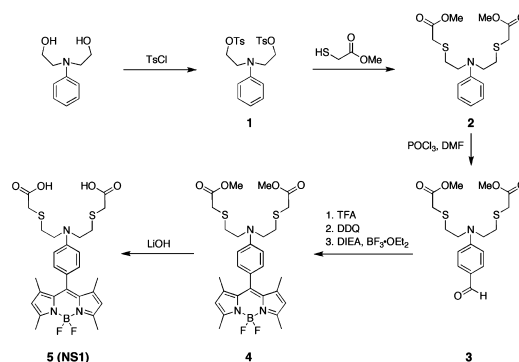

507 nm) compared to the apo probe. The turn-on response is reversible; treatment of Ni²⁺-loaded NS1 with the divalent metal ion chelator TPEN restores NS1 fluorescence back to baseline levels. A Hill plot indicates a simple binding process with no cooperativity (Figure S1a), and the apparent K_d for Ni²⁺ binding to NS1 is $193 \pm 5 \mu\text{M}$ (Figure S1b).

NS1 exhibits a selective turn-on fluorescence response to Ni²⁺ in water. Responses of 2 μM NS1 to the presence of various biologically relevant metal ions are shown in Figure 1b. The fluorescence profiles of apo or Ni²⁺-bound NS1 are unchanged in the presence of 1 mM Na⁺, K⁺, Mg²⁺, and Ca²⁺, indicating excellent selectivities for Ni²⁺ over these alkali and alkaline earth cations. Moreover, a series of 3d divalent metal cations, including 100 μM Mn²⁺, Fe²⁺, Co²⁺, and Zn²⁺, do not trigger NS1 fluorescence enhancements or interfere with the Ni²⁺ response. Of the first-row divalent transition metal ions, Cu²⁺ at 100 μM can mute the turn-on Ni²⁺ response of NS1, but lower Cu²⁺ levels (2 μM) minimize this interference. As expected, Cu²⁺ binds the sensor due to Irving–Williams series considerations, but the paramagnetic d⁹ ion quenches fluorescence, suggesting that the fluorescence increase observed for Ni²⁺ is due to a diamagnetic d⁸ state.

We next established the ability of NS1 to track Ni²⁺ levels in living cells using a model for respiratory nickel exposure. Live-cell confocal microscopy imaging experiments utilized the acetoxymethyl ester form of NS1 (NS1-AM) to enhance membrane permeability. Live human lung carcinoma A549 cells loaded with a 1:1 (v/v) mixture of NS1-AM and Pluronic F-127 (10 μM) for 35 min at 37 °C show weak intracellular fluorescence (Figure 2a). A549 cells supplemented with 1 mM NiCl₂ in the growth medium for 18 h at 37 °C and then stained with NS1 under the same loading conditions results in an increase in observed intracellular fluorescence intensity (Figure 2b); previous experiments establish that this exposure level of nickel is not lethal to lung carcinoma cells, whereas 2–10 mM Ni²⁺ causes widespread cell death.³⁵ Treatment of cells loaded with NS1 and Ni²⁺ with the divalent metal chelator TPEN (1 mM) for 1 min at 25 °C reverses the observed fluorescence increases (Figure 2c). Finally, Hoescht-3342 staining confirms that

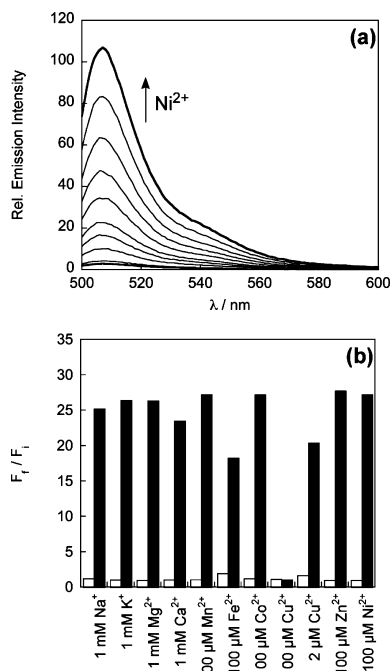


Figure 1. (a) Fluorescence response of 2 μM NS1 to Ni^{2+} . Spectra shown are for Ni^{2+} concentrations of 0, 2, 5, 10, 15, 25, 35, 50, 75, 100 μM . Spectra were acquired in 20 mM HEPES, pH 7.1, with 488 nm excitation. (b) Fluorescence responses of 2 μM NS1 to various metal ions. Bars represent the final (F_i) over the initial (F_x) integrated emission. Spectra were acquired in HEPES, pH 7.1. White bars represent the addition of the competing metal ion to a 2 μM solution of NS1. Black bars represent addition of 100 μM Ni^{2+} to the solution. Excitation was provided at 488 nm, with emission integrated over 498–700 nm.

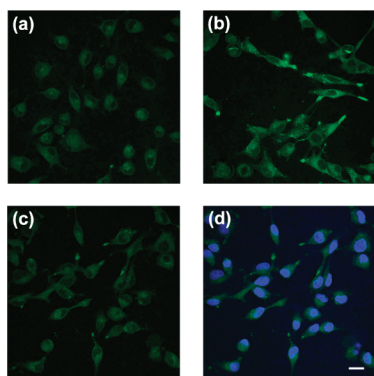


Figure 2. Live-cell imaging of intracellular Ni^{2+} levels by confocal microscopy. (a) Control A549 cells incubated with a 1:1 mixture of 10 μM NS1-AM and Pluronic F-127 for 35 min at 37 $^{\circ}\text{C}$. (b) Cells supplemented with 1 mM NiCl_2 in the growth medium for 18 h at 37 $^{\circ}\text{C}$ and stained with 10 μM NS1-AM and Pluronic F-127 for 35 min at 37 $^{\circ}\text{C}$. (c) NS1-loaded, 1 mM Ni^{2+} -supplemented cells treated with 1 mM of the divalent metal chelator TPEN for 1 min at 25 $^{\circ}\text{C}$. (d) NS1-loaded, 1 mM Ni^{2+} -supplemented cells treated with 1 mM TPEN, stained with 5 μM Hoescht-3342 to show cell viability. Scale bar = 20 μm .

the cells are viable throughout the imaging studies (Figure 2d). These data establish that NS1 can respond to changes in intracellular Ni^{2+} levels within living cells.

In closing, we have described the synthesis, spectroscopy, and application of NS1, a new fluorescent sensor for Ni^{2+} in biological samples. NS1 is a unique Ni^{2+} -responsive small-molecule indicator that features visible excitation and emission profiles and a selective turn-on response to Ni^{2+} compared to other biologically relevant

metal ions. Confocal microscopy experiments show that NS1 can be used for detecting changes in Ni^{2+} levels within living cells. Future plans will focus on improving the optical brightness and binding affinities of this first-generation probe as well as applying NS1 and related chemical tools to probe the cell biology of nickel.

Acknowledgment. We thank the Dreyfus, Packard, and Sloan Foundations, the Hellman Faculty Fund, Amgen, NSF (CAREER CHE-0548245), NIH (GM 79465), and HHMI for providing funding for this work. We thank Holly Aaron (UCB Molecular Imaging Center) and Ann Fischer and Michelle Yasukawa (UCB Tissue Culture Facility) for expert technical assistance.

Supporting Information Available: Synthetic and experimental details. This material is available free of charge via the Internet at <http://pubs.acs.org>.

References

- (1) Sigel, A.; Sigel, H.; Sigel, R. K. O., Eds. *Nickel and Its Surprising Impact in Nature*; John Wiley & Sons Ltd.: U.K., 2007; Vol. 2.
- (2) Chivers, P. T.; Sauer, R. T. *Protein Sci.* **1999**, *8*, 2494–2500.
- (3) Dosanjh, N. S.; Michel, S. L. *Curr. Opin. Chem. Biol.* **2006**, *10*, 123–130.
- (4) Giedroc, D. P.; Arunkumar, A. I. *Dalton Trans.* **2007**, 3107–3120.
- (5) Hausinger, R. P.; Zamble, D. B. In *Molecular Microbiology of Heavy Metals*; Nies, D. H., Silver, S., Eds.; Springer: Heidelberg, Germany, 2007; pp 287–320.
- (6) Wang, S. C.; Dias, A. V.; Zamble, D. B. *Dalton Trans.* **2009**, 2459–2466.
- (7) Carrington, P. E.; Chivers, P. T.; Al-Mjeni, F.; Sauer, R. T.; Maroney, M. J. *Nat. Struct. Biol.* **2003**, *10*, 126–130.
- (8) Schreiter, E. R.; Sintchak, M. D.; Guo, Y.; Chivers, P. T.; Sauer, R. T.; Drennan, C. L. *Nat. Struct. Biol.* **2003**, *10*, 794–799.
- (9) Phillips, C. M.; Schreiter, E. R.; Guo, Y.; Wang, S. C.; Zamble, D. B.; Drennan, C. L. *Biochemistry* **2008**, *47*, 1938–1946.
- (10) Iwig, J. S.; Leitch, S.; Herbst, R. W.; Maroney, M. J.; Chivers, P. T. *J. Am. Chem. Soc.* **2008**, *130*, 7592–7606.
- (11) Maroney, M. J. *Curr. Opin. Chem. Biol.* **1999**, *3*, 188–199.
- (12) Drennan, C. L.; Doukov, T. I.; Ragsdale, S. W. *J. Biol. Inorg. Chem.* **2004**, *9*, 511–515.
- (13) Evans, D. J. *Coord. Chem. Rev.* **2005**, *249*, 1582–1595.
- (14) Fontecilla-Camps, J. C.; Volbeda, A.; Cavazza, C.; Nicolet, Y. *Chem. Rev.* **2007**, *107*, 4273–4303.
- (15) Lindahl, P. A. *Angew. Chem., Int. Ed.* **2008**, *47*, 4054–4056.
- (16) Ragsdale, S. W. *J. Biol. Chem.* **2009**, *284*, 18571–18575.
- (17) Xia, W.; Li, H.; Sze, K. H.; Sun, H. J. *Am. Chem. Soc.* **2009**, *131*, 10031–10040.
- (18) Goodman, J. E.; Prueitt, R. L.; Dodge, D. G.; Thakali, S. *Crit. Rev. Toxicol.* **2009**, *39*, 365–417.
- (19) Costa, M.; Davidson, T. L.; Chen, H.; Ke, Q.; Zhang, P.; Yan, Y.; Huang, C.; Kluz, T. *Mutat. Res.* **2005**, *592*, 79–88.
- (20) Nemec, A. A.; Leikauf, G. D.; Pitt, B. R.; Wasserloos, K. J.; Barchowsky, A. *Am. J. Respir. Cell Mol. Biol.* **2009**, *41*, 69–75.
- (21) Domaille, D. W.; Que, E. L.; Chang, C. J. *Nat. Chem. Biol.* **2008**, *4*, 168–175.
- (22) Que, E. L.; Domaille, D. W.; Chang, C. J. *Chem. Rev.* **2008**, *108*, 1517–1549.
- (23) Torrado, A.; Walkup, G. K.; Imperiali, B. *J. Am. Chem. Soc.* **1998**, *120*, 609–610.
- (24) Pearce, D. A.; Walkup, G. K.; Imperiali, B. *Bioorg. Med. Chem. Lett.* **1998**, *8*, 1963–1968.
- (25) Salins, L. L.; Goldsmith, E. S.; Ensor, C. M.; Daunert, S. *Anal. Bioanal. Chem.* **2002**, *372*, 174–180.
- (26) Wang, B. Y.; Hu, Y. L.; Su, Z. X. *React. Funct. Polym.* **2008**, *68*, 1137–1143.
- (27) Wang, B. Y.; Liu, X. Y.; Hu, Y. L.; Su, Z. X. *Polym. Int.* **2009**, *58*, 703–709.
- (28) Fabbri, L.; Licchelli, M.; Pallavicini, P.; Perotti, A.; Taglietti, A.; Sacchi, D. *Chem.—Eur. J.* **1996**, *2*, 75–82.
- (29) Bolletta, F.; Costa, I.; Fabbri, L.; Licchelli, M.; Montalti, M.; Pallavicini, P.; Prodi, L.; Zaccheroni, N. *J. Chem. Soc., Dalton Trans.* **1999**, 1381–1385.
- (30) Jiang, L. J.; Luo, Q. H.; Wang, Z. L.; Liu, D. J.; Zhang, Z.; Hu, H. W. *Polyhedron* **2001**, *20*, 2807–2812.
- (31) Ke, Q.; Davidson, T.; Kluz, T.; Oller, A.; Costa, M. *Toxicol. Appl. Pharmacol.* **2007**, *219*, 18–23.
- (32) Thierse, H. J.; Helm, S.; Pink, M.; Weltzien, H. U. *J. Immunol. Methods* **2007**, *328*, 14–20.
- (33) Zhao, J.; Bertoglio, B. A.; Devinney, M. J., Jr.; Dineley, K. E.; Kay, A. R. *Anal. Biochem.* **2009**, *384*, 34–41.
- (34) Cadosch, D.; Meagher, J.; Gautschi, O. P.; Filgueira, L. J. *Neurosci. Methods* **2009**, *178*, 182–187.
- (35) Chen, H.; Costa, M. *Exp. Biol. Med.* **2006**, *231*, 1474–1480.

JA906500M