


RSC Advances



This article can be cited before page numbers have been issued, to do this please use: L. Lu, Q. Gao, C. Song, X. Tian and A. Xu, *RSC Adv.*, 2014, DOI: 10.1039/C4RA04552A.




This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. This *Accepted Manuscript* will be replaced by the edited, formatted and paginated article as soon as this is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

Graphic Abstract:



A novel and environmentally friendly strategy based on unmodified AuNPs was developed for the colorimetric detection of cysteine in human urine.

Cite this: DOI: 10.1039/c0xx00000x

www.rsc.org/xxxxxx

ARTICLE TYPE

A novel and environmentally friendly colorimetric method for detection of cystine in human urine using unmodified gold nanoparticles

Li-Qiang Lu,^{*a} Qian Gao,^a Chi Song,^a Xi-Ke Tian^a and An-Wu Xu^b

Received (in XXX, XXX) Xth XXXXXXXXX 20XX, Accepted Xth XXXXXXXXX 20XX

DOI: 10.1039/b000000x


Cystine was reduced by ascorbic acid to cysteine, which induced the aggregation of unmodified gold nanoparticles. The accompanied color change was distinguishable and perceivable by the naked eye. This facile assay method was successfully applied to the detection of cystine in human urine.

Cystinuria is a congenital metabolic disease, which stems from the defective transport of cystine and dibasic amino acids through the epithelial cells of the renal tubule and intestinal tract, resulting in the recurrent formation of cystine stones in the renal tract.^[1] Cystinuria could be characterized by high concentrations of cystine in human urine (usually >400 mg L⁻¹).^[2] Several methods for the analysis of cystine have been developed during the past decades, including iodimetry,^[3] liquid chromatography,^[4] electrochemistry,^[5-7] spectrophotometry,^[8,9] spectrofluorimetry^[10] and colorimetry.^[11-13] Among these methods, colorimetric assay is most attractive, especially in a resource poor setting, due to its simplicity and no requirement for sophisticated instruments. The traditional colorimetric cystine detection are based on the reaction between cysteine and nitroprusside,^[12] where cysteine is reduced from cystine by potassium cyanide. Although this assay has been used for clinical analysis of cystine in human urine, it suffers from high blanks, unstable colors, low specificity, high sensitivity to reaction conditions, and toxicity of reductant.^[13] On the basis of the aforementioned facts, it is desirable to develop sensors that provide sensitive, specific and environmentally friendly detection of cystine.

Gold nanoparticles (AuNPs) have been demonstrated to be suitable for colorimetric sensors, owing to their unique optical properties related to surface plasmon resonance (SPR).^[14,15] A vast variety of AuNPs-based colorimetric sensors have been exploited to detect DNA,^[16] proteins^[17] and small molecules^[18-22]. Thereinto, cetyltrimethylammonium bromide capped AuNPs,^[18] fluorosurfactant stabilized AuNPs^[19] and unmodified AuNPs^[20] were used for sensing cysteine. However, as far as we are aware, AuNPs-based colorimetric methods have not yet been applied for the detection of cystine.

Herein, we present a facile, rapid and sensitive colorimetric method based on unmodified AuNPs for the assay of cystine. As shown in Scheme 1, cystine which cannot induce the aggregation of AuNPs is reduced by ascorbic acid to cysteine that can readily bind to the surface of AuNPs via Au-S bond. Consequently, the AuNPs aggregation occurs due to the electrostatic interaction

between the positively charged amino group and the negatively charged carboxyl group of cysteine on the surface of AuNPs, with a corresponding red to blue color change which can be easily observed by the naked eye or measured with ultraviolet-visible (UV-Vis) spectroscopy.



Scheme 1 Schematic illustration of the strategy for the colorimetric assay of cystine based on unmodified AuNPs and ascorbic acid.

AuNPs with ~18 nm in diameter were synthesized by citrate reduction of HAuCl₄ (ESI, Experimental section) as previously reported,^[23] exhibiting a SPR absorption band peaked at 520 nm (Fig. 1A, black curve). The AuNPs solution could be stabilized against aggregation ascribed to the electrostatic repulsion between citrate capped AuNPs. In the presence of cystine, only a very slight decrease in the SPR absorption band of AuNPs was observed (Fig. 1A, blue curve), and the solution color remained red (Fig. 1B, left), indicating that AuNPs did not aggregate, which was also demonstrated by TEM observation (Fig. 1C). However, it has been previously discussed that cysteine can induce the aggregation of AuNPs because of the covalent bonding to AuNPs via the mercapto group and the electrostatic interaction between cysteine zwitterions on the surface of neighboring AuNPs.^[24] Accordingly, we designed our AuNPs-based colorimetric method to indirectly detect cystine by reducing cystine to cysteine. Ascorbic acid was chosen as the reductant since it can reduce the poorly soluble cystine to the readily soluble cysteine and has been used to treat cystinuria.^[25] In the cystine detection case, cystine (10 μM) was mixed with ascorbic acid (2 mM) and incubated at 40 °C for 15 min, and then

AuNPs (0.5 ml) were added (ESI, Experimental section). The SPR peak at 520 nm significantly decreased and a new distinct SPR peak at 670 nm appeared (Fig. 1A, green curve), showing the aggregation of AuNPs, which was confirmed by TEM image (Fig. 1D). The solution color change from red to blue was distinguishable and perceivable by the naked eye (Fig. 1B, right). The control experiment showed that ascorbic acid (2 mM) had no effect on the stability of AuNPs (Fig. 1A, red curve). Therefore, it is convenient to probe cystine through the color change and absorption spectra of AuNPs solutions.




Fig. 1 Absorption spectra (A), optical photographs (B) and TEM images (C and D) of AuNPs in the presence of cystine and in the presence of the reaction mixture of cystine and ascorbic acid.

To achieve better analysis performance, optimizations of some key variables of cystine measurement were conducted, where the relative absorbance A_{650}/A_{520} that is the ratio of the extinction coefficients at 650 nm and 520 nm was used to express the molar ratio of the aggregated to the dispersed AuNPs. The amount of AuNPs was optimized to 0.5 ml where the ratio of A_{650}/A_{520} reaches its maximum (ESI, Fig. S1). The concentration of the ascorbic acid, reaction temperature and reaction time of cystine reduction were optimized to 2 mM (ESI, Fig. S2), 40 °C (ESI, Fig. S3) and 15 min, respectively, for further experiments.

Under the optimum conditions, different concentrations of cystine were tested and UV-Visible spectra of the solutions were recorded. As shown in Fig. 2A, absorbance at 520 nm decrease while absorbance at 650 nm increase with sequentially increasing concentrations of aliquots of cystine. The ratios of A_{650}/A_{520} is linearly related to the cystine concentrations ranging from 1 μM to 8 μM , and the calibration equation, $A=0.18055c-0.04126$, is obtained with a correlation coefficient of 0.991 (Fig. 2B). In addition, Fig. 2C clearly shows that the color of AuNPs solution is gradually changed from wine red to blue with the increase of cystine concentration. The detection limit of cystine is down to 1 μM with the naked eye, which is much better than the previously reported electrochemical^[5] and colorimetric^[13] determination of cystine. The result indicates that the proposed assay method can

conveniently determine cystine with high sensitivity.

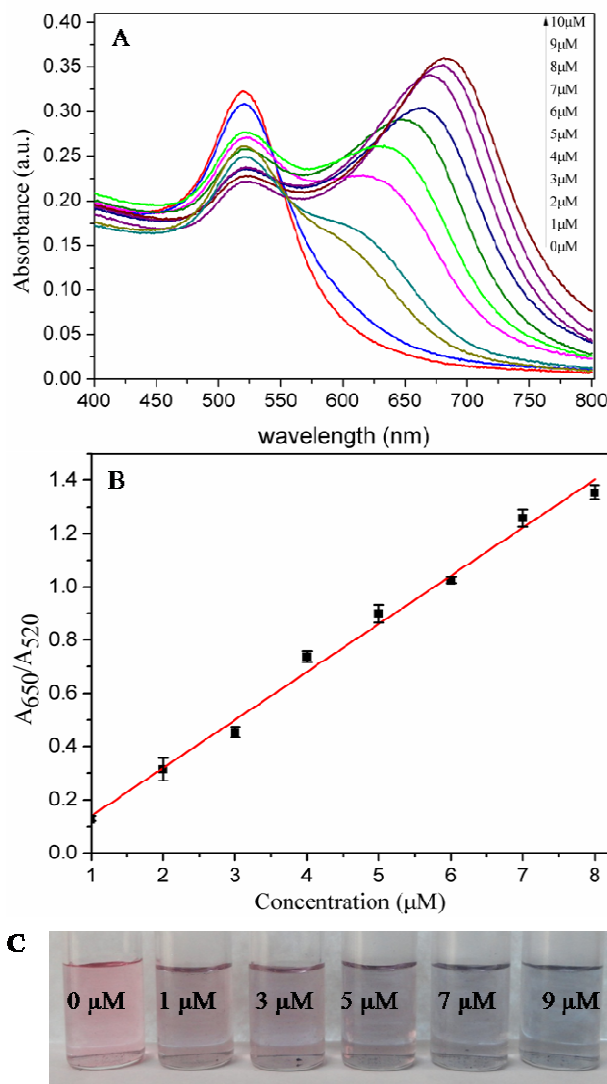


Fig. 2 (A) Absorbance response for different concentrations of cystine. (B) Calibration curve for the detection of cystine. The error bars denote standard deviation from three independent measurements. (C) Color change of AuNPs solution with the increase of cystine concentration.

Several other substances perhaps existing in the urine were employed to assess the selectivity of the present colorimetric cystine assay method. As illustrated in Fig. 3A, cystine, homocysteine and cysteine result in red-to-blue color changes while the solutions remain red in the presence of other objects. The corresponding relative absorbance data show that other substances cause a negligible increase of A_{650}/A_{520} at a 2-fold molar excess (Fig. 3C). As known in previous reports, the concentrations of cysteine (98±35 $\mu\text{mol/L}$) in urine from cystinurics are much lower than that of cystine (1185±451 $\mu\text{mol/L}$),^[26] and the homocysteine is normally found at relatively low concentration (2-14 $\mu\text{mol/L}$) in human urine.^[27] Therefore, the interference of cysteine and homocysteine could be ignored in diluted patients urine sample. In coexistence interference experiments, only iodide makes a decrease of absorption ratio value (Fig. 3D) with a purple solution (Fig. 3B). It is known that the concentrations of iodide in healthy human urine are about

86.8±19.0 µg/L.^[28] Thus, the interference of iodide could also be ignored in urine samples from cystinurics.




Fig. 3 (A) Color change of AuNPs solution in the presence of 10 µM cystine or 20 µM other substances. (B) Color change of AuNPs solution in the presence of 10 µM cystine and 20 µM other substances. (C) The relative absorption value for 10 µM cystine or 20 µM other substances. (D) The relative absorption value for 10 µM cystine and 20 µM other substances.

Based on the positive results, we next studied the application of the colorimetric assay method in real urine samples. Prior to analysis, the urine sample was diluted 1:100 (v/v) with deionized

water to avoid the aggregation of AuNPs induced by the high concentration of ions, protein and small molecules. A series of obtained urine samples were prepared by spiking them with standard solution of cystine over the range from 1 µM to 9 µM.

The measuring results of cystine in urine samples were shown in Fig. 4A. There is a good linear relationship between the ratio of A_{650}/A_{520} and the concentration of cystine with a correlation coefficient of 0.995 (Fig. 4B). The lowest detectable concentration of cystine in urine sample was also 1 µM. Validation of the proposed method was examined by spiking urine samples collected from two healthy children (Volunteer I: 0.5 years old, Volunteer II: 2 years old) with cystine concentrations of 2 µM, 5 µM and 8 µM. The analytical results for the urine samples are shown in table 1. As can be seen in table 1, the recoveries of cystine range from 99.5 % to 106.8 % with RSDs ranging from 1.27 % to 5.74 %, thereby proving that this colorimetric assay is an accurate and sensitive method for the analysis of cystine in human urine.

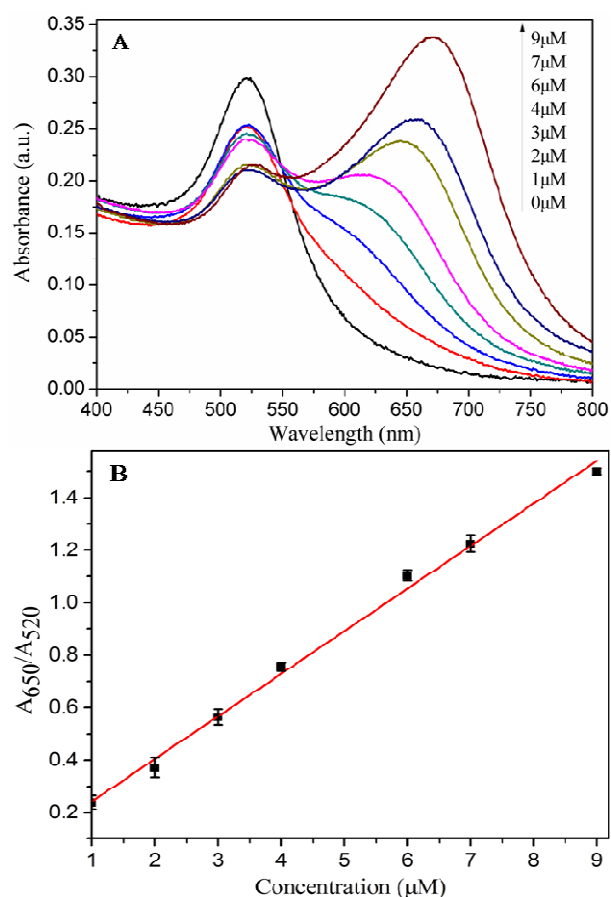


Fig. 4 (A) Absorbance response for different concentrations of cystine in urine sample. (B) Calibration curve for the detection of cystine. The error bars denote standard deviation from three independent measurements.

Table 1 Determination of cystine in real urine samples and recovery test

Sample	Added (µM)	Detected (µM)	Recovery (%)	RSD (%; n=6)
Volunteer I	2	1.994	99.7	3.43
Volunteer II	2	2.079	101	3.02

Volunteer I	5	4.975	99.5	2.09
Volunteer II		5.34	106.8	5.74
Volunteer I	8	8.2	102.5	1.27
Volunteer II		8.29	103.6	2.12

In summary, we have developed a novel and simple strategy based on unmodified AuNPs for the colorimetric detection of cystine. Cystine is effectively reduced by nontoxic ascorbic acid to cysteine, inducing the aggregation of unmodified AuNPs through the efficient electrostatic interaction between cysteine-bonded AuNPs. The color detection limit of the proposed method is down to 1 μM with the naked eye, which is more sensitive than previously reported colorimetric methods. The practicability of this method was validated through analyses of real urine samples. Compared with the existing methods for measurement of cystine in human urine, the colorimetric assay method demonstrated here is advantageous in terms of its simplicity and nontoxicity, and is thus highly anticipated to assist in the diagnosis of human cystinuria.

The authors acknowledge the geological survey project of China Geological Survey (12120113015300) and the special funding support from the Fundamental Research Funds for the Central Universities (CUG090108).

Notes and references

^a Nano-Mineral Materials and Application Engineering Research Center of Ministry of Education, Faculty of Materials Science and Chemistry, China University of Geosciences, Wuhan 430074, P. R. China. E-mail: llqdic@cug.edu.cn

^b Division of Nanomaterials and Chemistry, Hefei National Laboratory for Physical Sciences at Microscale, Department of Chemistry, University of Science and Technology of China, Hefei 230026, P. R. China.

† Electronic Supplementary Information (ESI) available: experimental section and variables optimization. See DOI: 10.1039/b000000x/

‡ Footnotes should appear here. These might include comments relevant to but not central to the matter under discussion, limited experimental and spectral data, and crystallographic data.

1 M. J. Calonge, P. Gasparini, J. Chillarón, M. Chillón, M. Gallucci, F. Rousaud, L. Zelante, X. Testar, B. Dallapiccola, F. Di Silverio, P. Barceló, X. Estivill, A. Zorzano, V. Nunes and M. Palacín, *Nature Genetics*, 1994, 6, 420-425.

2 S. R. Karl and C. M. James, *Saudi J Kidney Dis Transplant*, 2003, 14 (1): 351-357.

3 R. W. Virtue and H. B. Lewis, *J. Biol. Chem.*, 1934, 104, 415.

4 Y. Wang, X. J. Kang and W. H. Ge, *Chromatographia*, 2007, 65, 527-532.

5 P. Mikus, P. Kubacak, I. Valaskova and E. Havranek, *Pharmazie*, 2003, 58, 111-113.

6 G. Li, J. Yang, X. Zheng, M. Meng and J. Cao, *Microchim Acta*, 2010, 168, 277-282.

7 M. S. Damle, L. A. A. Newton, M. M. Villalba, R. Leslie and J. Davis, *Electroanalysis*, 2010, 21, 2491-2495.

8 J. Chrastil, *Analyst*, 1989, 114, 1133-1136.

9 J. Chrastil, *Analyst*, 1990, 115, 1383-1384.

10 A. A. Ensafi, B. Rezaei and S. Nouroozi, *J. Braz. Chem. Soc.*, 2009, 2, 288-293.

11 Y. Morioka and K. Kobayashi, *Biol. Pharm. Bull.*, 1997, 20, 825-827.

12 I. W. Grote, *J. Biol. Chem.*, 1931, 93, 25-30.

13 K. Shinohara, *J. Biol. Chem.*, 1935, 109, 665-679.

14 M. Hu, J. Chen, Z. Li, L. Au, G.V. Hartland, X. Li, M. Marquez and Y. Xia, *Chem. Soc. Rev.*, 2006, 35, 1084-1094.

15 S. K. Ghosh and T. Pal, *Chem. Rev.*, 2007, 107, 4797-4862.

16 H. Li and L. J. Rothberg, *J. Am. Chem. Soc.*, 2004, 126, 10958-10961.

17 H. Wei, B. Li, J. Li, E. Wang and S. Dong, *Chem. Commun.*, 2007, 3735-3737.

18 J. Wang, Y. F. Li, C. Z. Huang and T. Wu, *Anal. Chim. Acta.*, 2008, 626, 37-43.

19 Q. Xiao, F. Shang, X. Xu, Q. Li, C. Lu and J.M. Lin, *Biosensors and Bioelectronics*, 2011, 30, 211-215.

20 L. Li and B. Li, *Analyst*, 2009, 134, 1361-1365.

21 G. Patel and S. Menon, *Chem. Commun.*, 2009, 3563-3565.

22 K. Ai, Y. Liu and L. Lu, *J. Am. Chem. Soc.*, 2009, 131, 9496-9497.

23 G. Frens, *Nature physical science*, 1973, 241, 20-22.

24 P. K. Sudeep, S. T. Shibu Joseph and K. George Thomas, *J. Am. Chem. Soc.*, 2005, 127, 6516-6517.

25 B. Lux, P. May, *Urol. Int.*, 1983, 38, 91-94.

26 H. Birwe and A. Hesse, *Clinica Chimica Acta*, 1991, 199, 33-42.

27 K. Kusmierek, R. Glowacki, and E. Bald, *Anal Bioanal Chem*, 2006, 385, 855-860.

28 J. L. Burguera, M. R. Brunetto, Y. Contreras, M. Burguera, M. Gallignani and P. Carrero, *Talanta*, 1996, 43, 839-850.