




Current Data Parameters
NAME RFS-QJHHSS-A-H1-DMSO-20180807
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20180807
Time 15.55
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8223.685 Hz
FIDRES 0.125483 Hz
AQ 3.9846387 sec
RG 197.41
DW 60.800 usec
DE 8.00 usec
TE 296.3 K
D1 1.0000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 1H
P1 13.22 usec
PLW1 15.84899998 W
SFO1 400.1632013 MHz

F2 - Processing parameters
SI 65536
SF 400.1600024 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

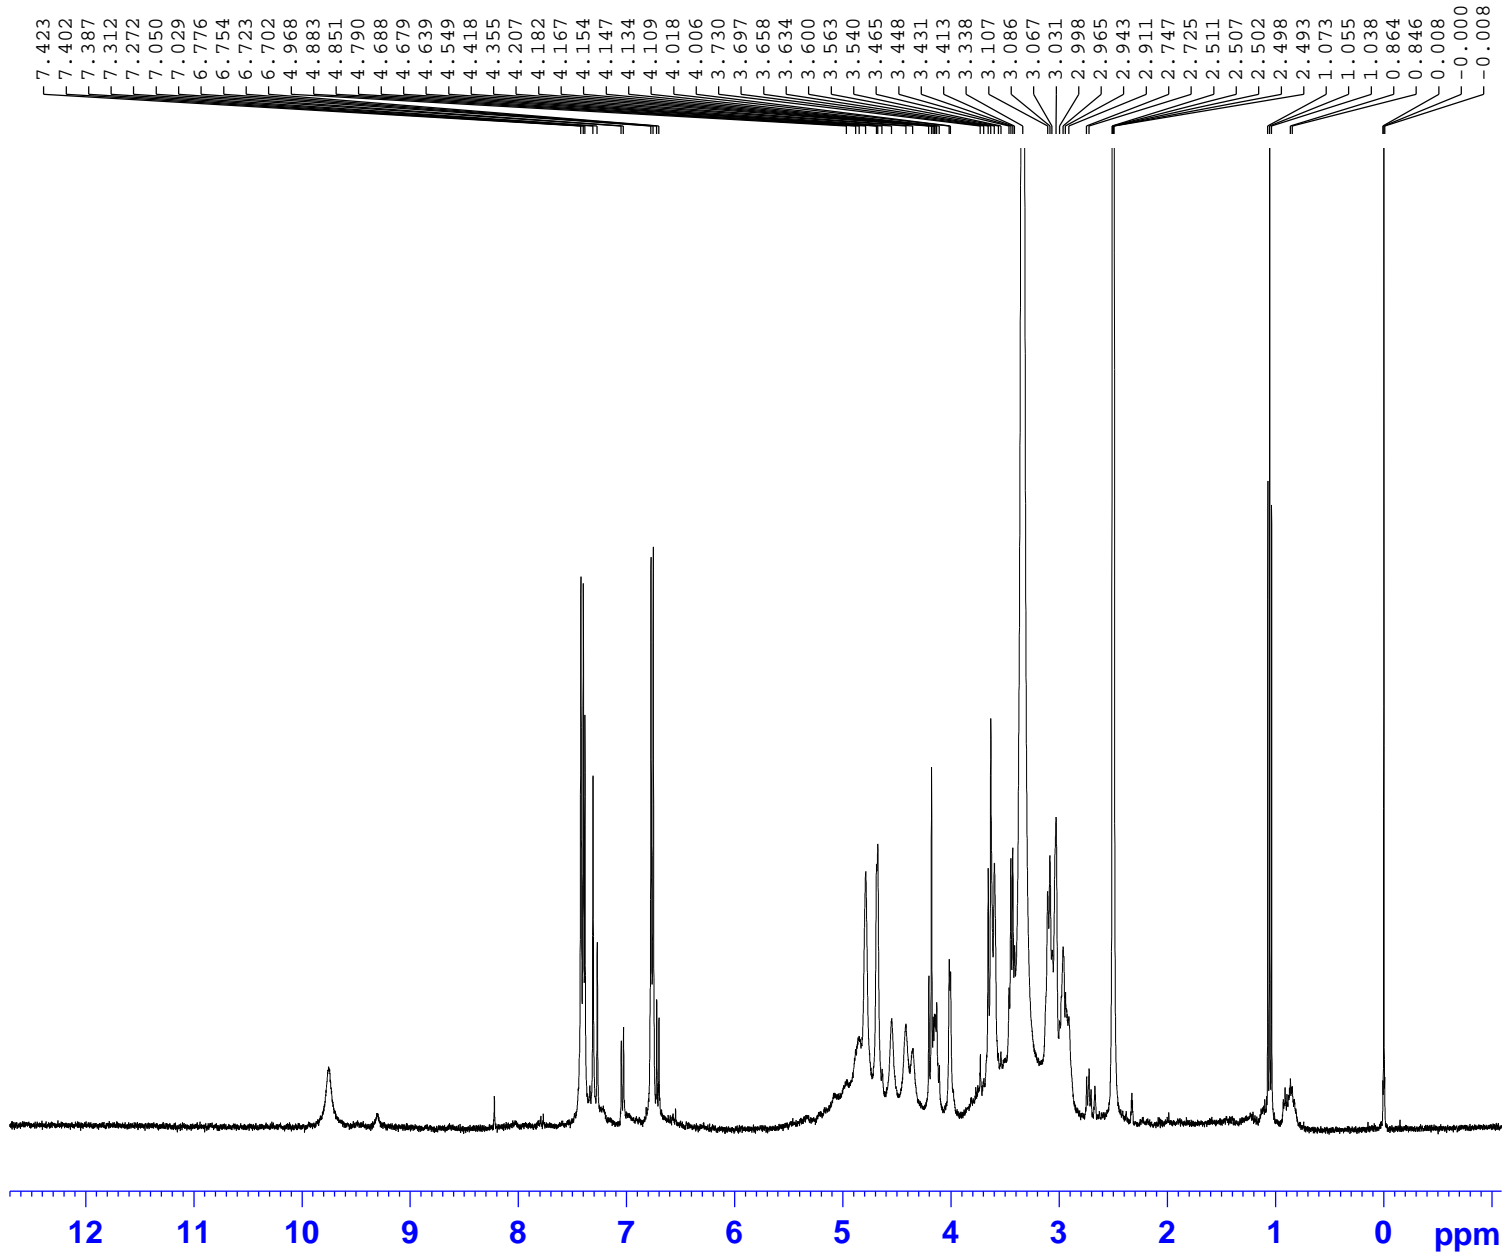

0.9791

3.2683
1.8082
0.4541
3.0048

3.0338
5.1663
1.3873
2.0542
1.2255
1.2715
1.2635
5.1354
2.8321
5.9350
3.1174

2.0000
0.7486