


**Data file:** E:\DATA\190821\MBCP021 19082003Final.D  
**Sample name:** MBCP021 19082003Final  
**Description:** Mobile phase: Buffer A:0.1%TFA in H2O  
 Buffer B:0.1%TFA in ACN  
 Gradient: 7-17% in 20min, Flow rate:1.0ml/min  
 Column:Unitary C18,4.6\*150mm, 5um 100A (A-001)  
 Instrument:Agilent HPLC 1100

**Instrument:** QC **Location:** 54  
**Injection date:** 2019/8/21 15:30:06 **Injection:** 1 of 1  
**Last changed:** 2019/8/21 16:16:11 **Injection volume:** 3.000  
**Acq. operator:** QC\_1

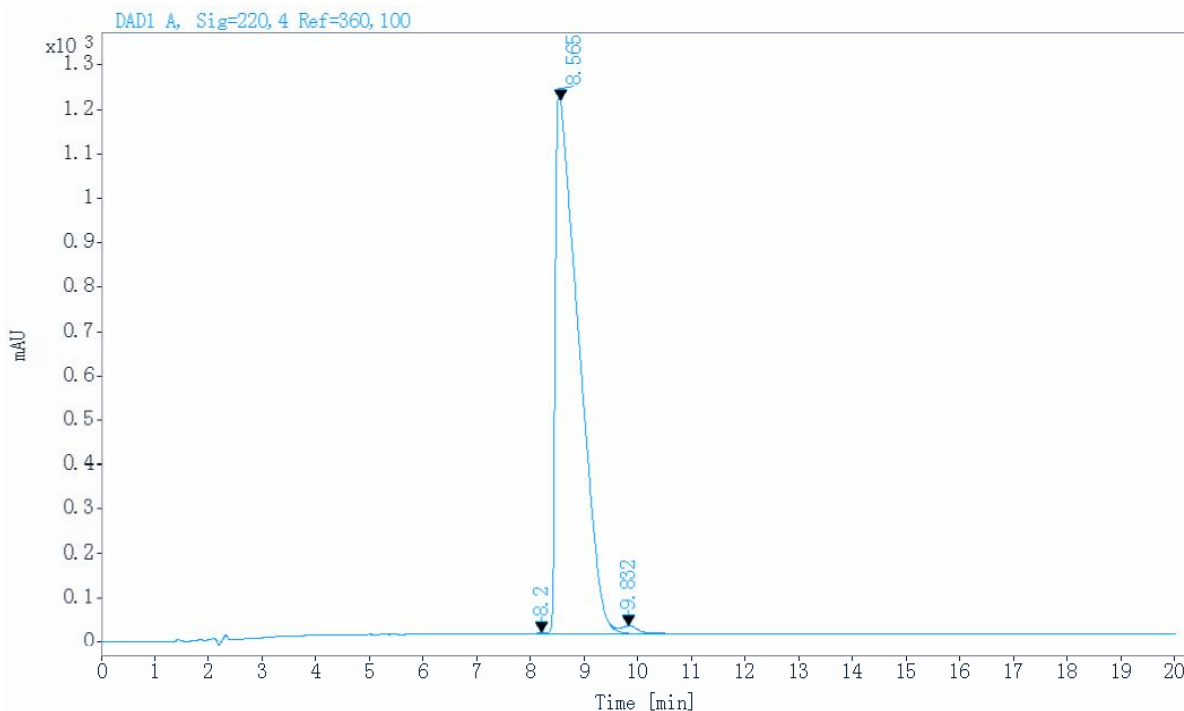

**Signal:** DAD1 A, Sig=220,4 Ref=360,100

RT[min]	Type	Width[min]	Area	Height	Area% Name
8.200	VV f	0.1084	6.5894	0.9109	0.0179
8.565	BV R	0.4768	36433.5039	1191.3597	98.8688
9.832	VB E	0.3573	410.2668	16.7790	1.1133
Sum			36850.3601		