


MOBEL BIOMATERIALS TECHNOLOGY CO.,LIMITED

OFFICE ADD: NO. 479 MINHE ROAD, NINGWEI STREET, XIAOSHAN DISTRICT, HANGZHOU CITY, CHINA. 311200
 TEL:+86-571-85099223 FAX: +86-571-85099222

Data file: E:\DATA\20072305\CP10028 Final.D
Sample name: CP10028 Final
Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient 52-62% in 20min, Flow rate: 1.0ml/min
 Column: Unitary C18, 4.6*150mm, 5um 100A (A-001)
 Instrument: Agilent HPLC 1100

Instrument: QC **Location:** 51
Injection date: 2020/7/25 12:12:26 **Injection:** 1 of 1
Last changed: 2020/7/25 12:35:08 **Injection volume:** 15.000
Acq. operator: QC_1

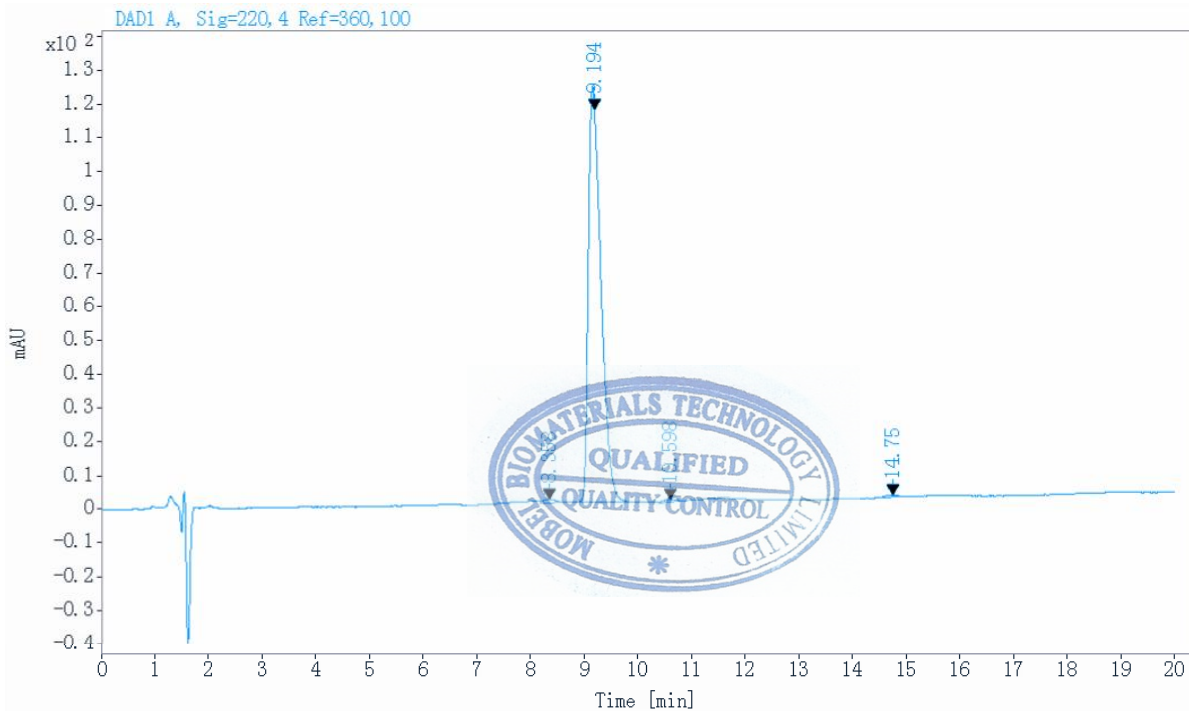

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area% Name
8.358	VB	0.2742	15.3733	0.9234	0.7518
9.194	BB	0.2857	2010.0187	114.0224	98.7105
10.598	MM	0.2136	9.0492	0.7062	0.4425
14.750	MM	0.2391	10.5359	0.7345	0.5152
Sum			2044.9771		