


Data file: E:\DATA\190323\20190323 2019-03-23 12-13-13\ CP100005 19032301 Final.D
Sample name: CP100005 19032301Final
Description: Mobile phase: Buffer A:0.1%TFA in H2O
 Buffer B:0.1%TFA in ACN
 Gradient: 45-55% in 20min, Flow rate:1.0ml/min
 Column:Unitary C18,4.6*150mm, 5um 100A (A-001)
 Instrument:Agilent HPLC 1100

Instrument: QC **Location:** 81
Injection date: 2019/3/23 12:17:16 **Injection:** 1 of 1
Last changed: 2019/3/23 13:47:21 **Injection volume:** 20.000
Acq. operator: QC_1

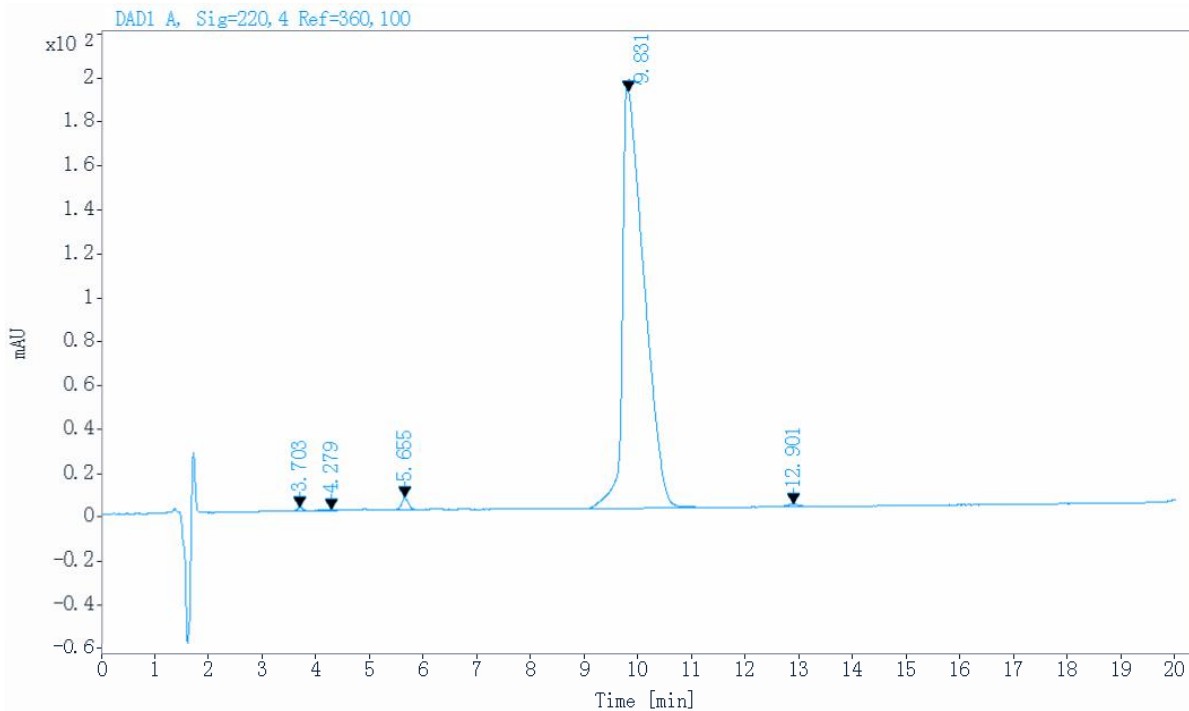

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area% Name
3.703	VV B	0.1466	15.3929	1.6845	0.2808
4.279	VV F	0.3495	5.7812	0.2124	0.1055
5.655	MM	0.1508	50.6004	5.5936	0.9230
9.831	BV R	0.4265	5389.7534	190.2328	98.3133
12.901	MM	0.2530	20.6934	1.3632	0.3775
Sum			5482.2214		