


Data file: E:\DATE\MCP0217 1Final.D
Sample name: MCP010 MCP0217 Final
Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in (40%ACN+60%H2O)
 Gradient: 15-40% in 20min
 Flow rate: 1.0ml/min
 Column: Unitary C18, 4.6*150mm, 5um 100A (A-001)
 Instrument: Agilent HPLC 1100

Instrument: QC **Location:** 71
Injection date: 2020/02/27 10:16:03 **Injection:** 1 of 1
Last changed: 2020/02/27 10:37:07 **Injection volume:** 20.000
Acq. operator: QC_1

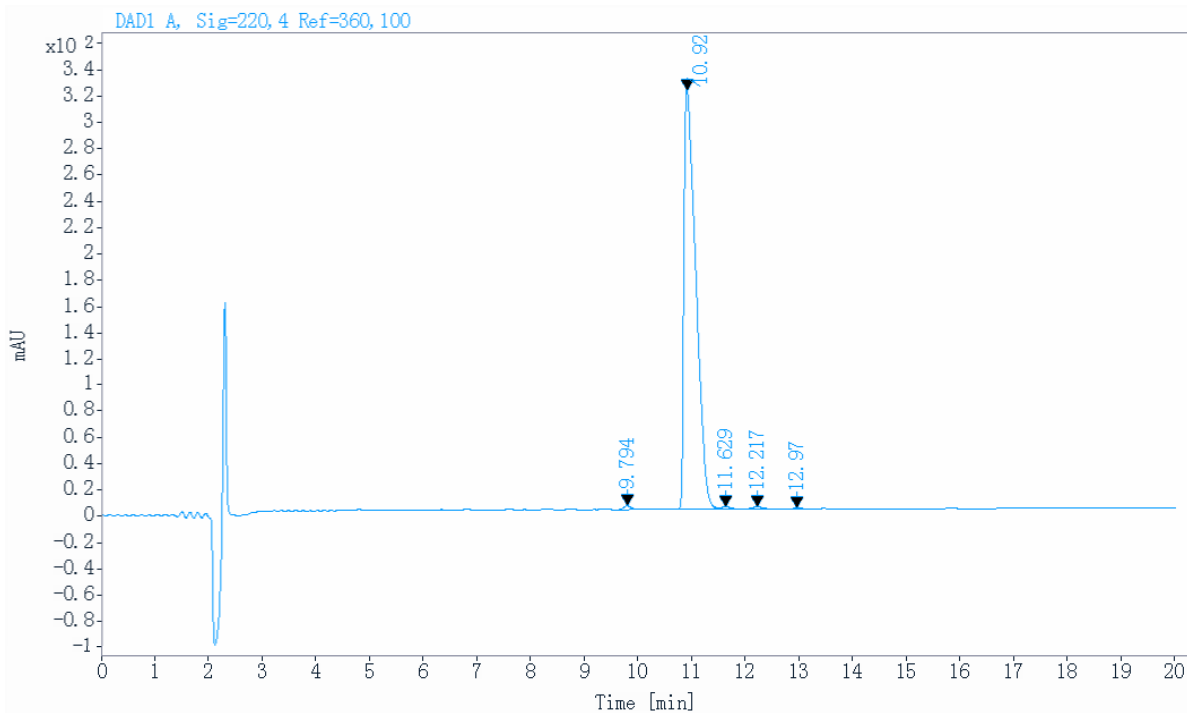

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
9.794	BB	0.1514	27.8896	2.9216	0.5573	
10.920	BV R	0.2424	4911.6201	321.2829	98.2312	
11.629	VV E	0.2162	23.9746	1.6625	0.4790	
12.217	VB E	0.1962	28.0611	2.0442	0.5607	
12.970	BBA	0.1624	13.0990	1.2094	0.2617	
Sum			5004.6445			