


**Data file:** E:\DATA\180702\100007\_19062903Final.D  
**Sample name:** 100007\_19062903Final  
**Description:** Mobile phase: Buffer A:0.1%TFA in H2O  
 Buffer B:0.1%TFA in ACN  
 Gradient 17-27% in 20min , Flow rate:1.0ml/min  
 Column:Unitary C18,4.6\*150mm, 5um 100A (A-001)  
 Instrument:Agilent HPLC 1100

**Instrument:** QC **Location:** 21  
**Injection date:** 2019/7/2 13:25:37 **Injection:** 1 of 1  
**Last changed:** 2019/7/2 13:54:28 **Injection volume:** 5.000  
**Acq. operator:** QC\_1

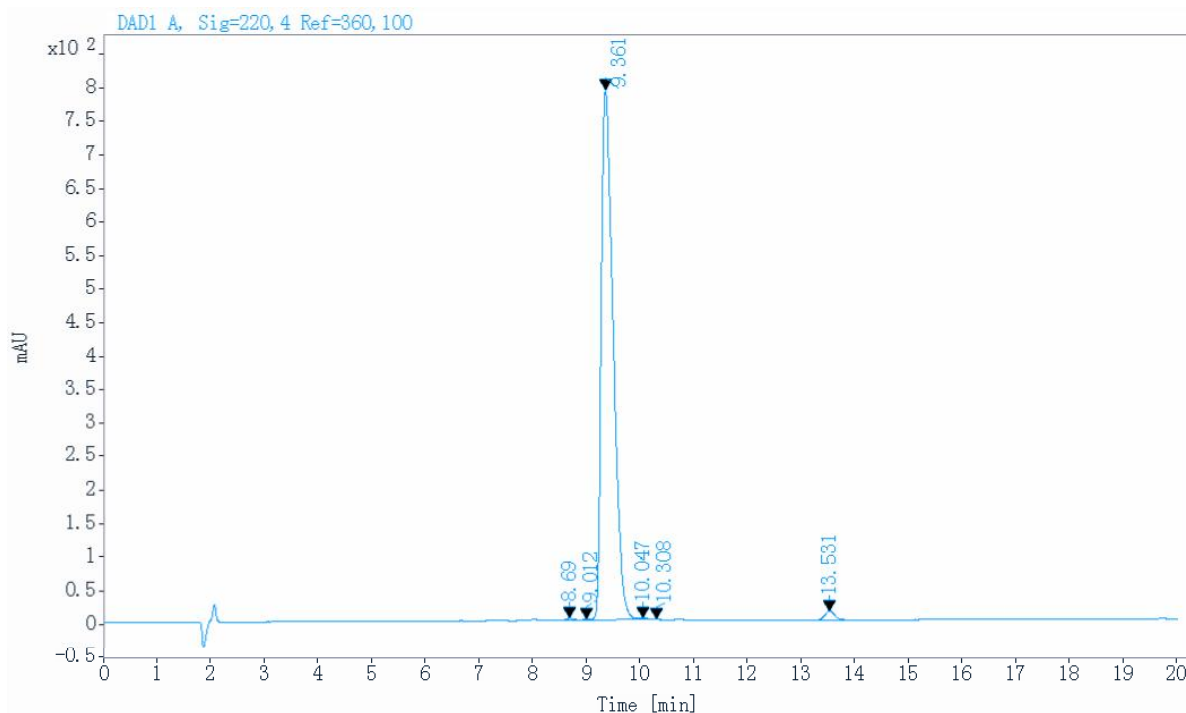

**Signal:** DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
8.690	VB R	0.1762	29.0947	2.6481	0.2346	
9.012	BV E	0.1359	10.4482	1.1736	0.0843	
9.361	VV R	0.2432	12154.7676	791.1741	98.0122	
10.047	VB E	0.1539	26.5573	2.7192	0.2141	
10.308	BB	0.1429	7.5700	0.8579	0.0610	
13.531	VV B	0.1954	172.8436	13.6827	1.3938	
Sum			12401.2815			