




7.366  
7.361  
7.355  
7.351  
7.345  
7.337  
7.323  
7.285  
7.205  
4.991  
4.961  
4.783  
4.753  
4.742  
4.713  
4.585  
4.578  
4.571  
4.566  
4.559  
4.555  
4.535  
4.505  
4.451  
4.432  
4.418  
4.134  
4.129  
4.120  
4.115  
3.707  
3.700  
3.680  
3.672  
3.597  
3.590  
3.569  
3.563

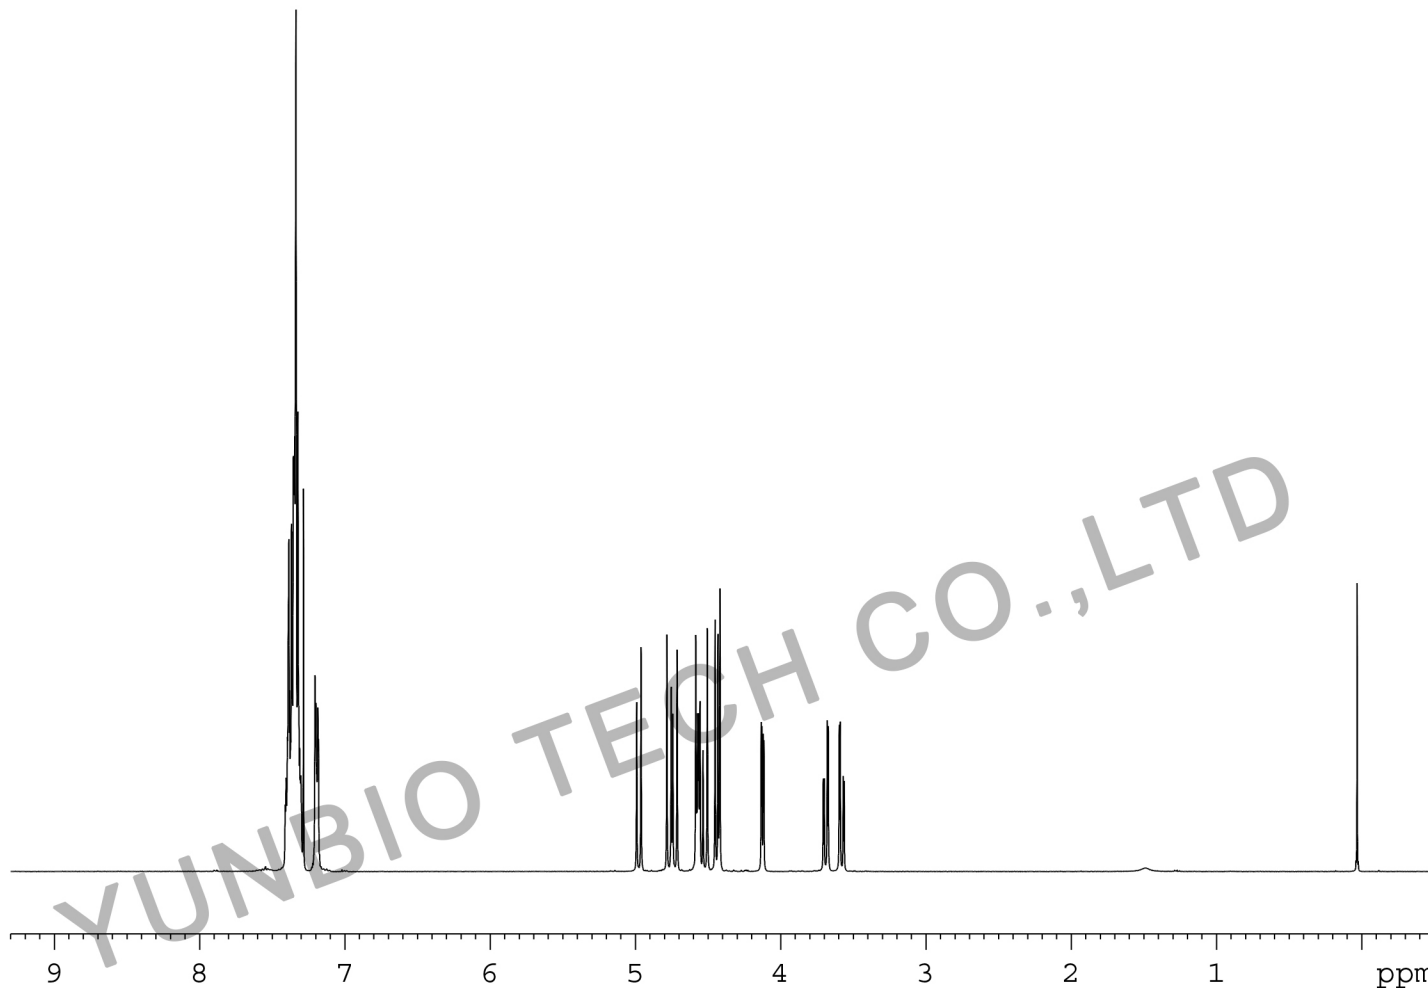

Current Data Parameters  
NAME MT05275  
EXPNO 13  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20190405  
Time 14.05  
INSTRUM spect  
PROBHD 5 mm PABBO BB-  
PULPROG zg30  
TD 65536  
SOLVENT CDC13  
NS 16  
DS 2  
SWH 8223.685 Hz  
FIDRES 0.125483 Hz  
AQ 3.9846387 sec  
RG 177.69  
DW 60.800 usec  
DE 6.50 usec  
TE 297.1 K  
D1 1.00000000 sec

===== CHANNEL f1 =====  
NUC1 1H  
P1 15.16 usec  
PLW1 13.99600029 W  
SFO1 400.1324710 MHz

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

12.70  
1.97  
1.01  
2.04  
3.03  
2.00  
1.00  
1.00  
1.00

YUNBIO TECH CO.,LTD