


Sample Name: 20220829-QC338568-567998

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :   44
Sample Operator : SYSTEM
Acq. Instrument : 8860                      Location  :   86 (F)
Injection Date  : 8/30/2022 12:00:02 AM      Inj       :    1
                                           Inj Volume: 1 µl
Acq. Method     : D:\ChemStation\1\Data\20211223\02 2022-08-29 14-14-15\20211224-280-.M
Last changed    : 8/29/2022 4:37:39 PM by SYSTEM
Analysis Method : D:\ChemStation\1\Data\20211223\02 2022-08-29 14-14-15\20211224-280-.M (
                  Sequence Method)
Last changed    : 8/30/2022 9:27:38 AM by SYSTEM
                  (modified after loading)
    
```

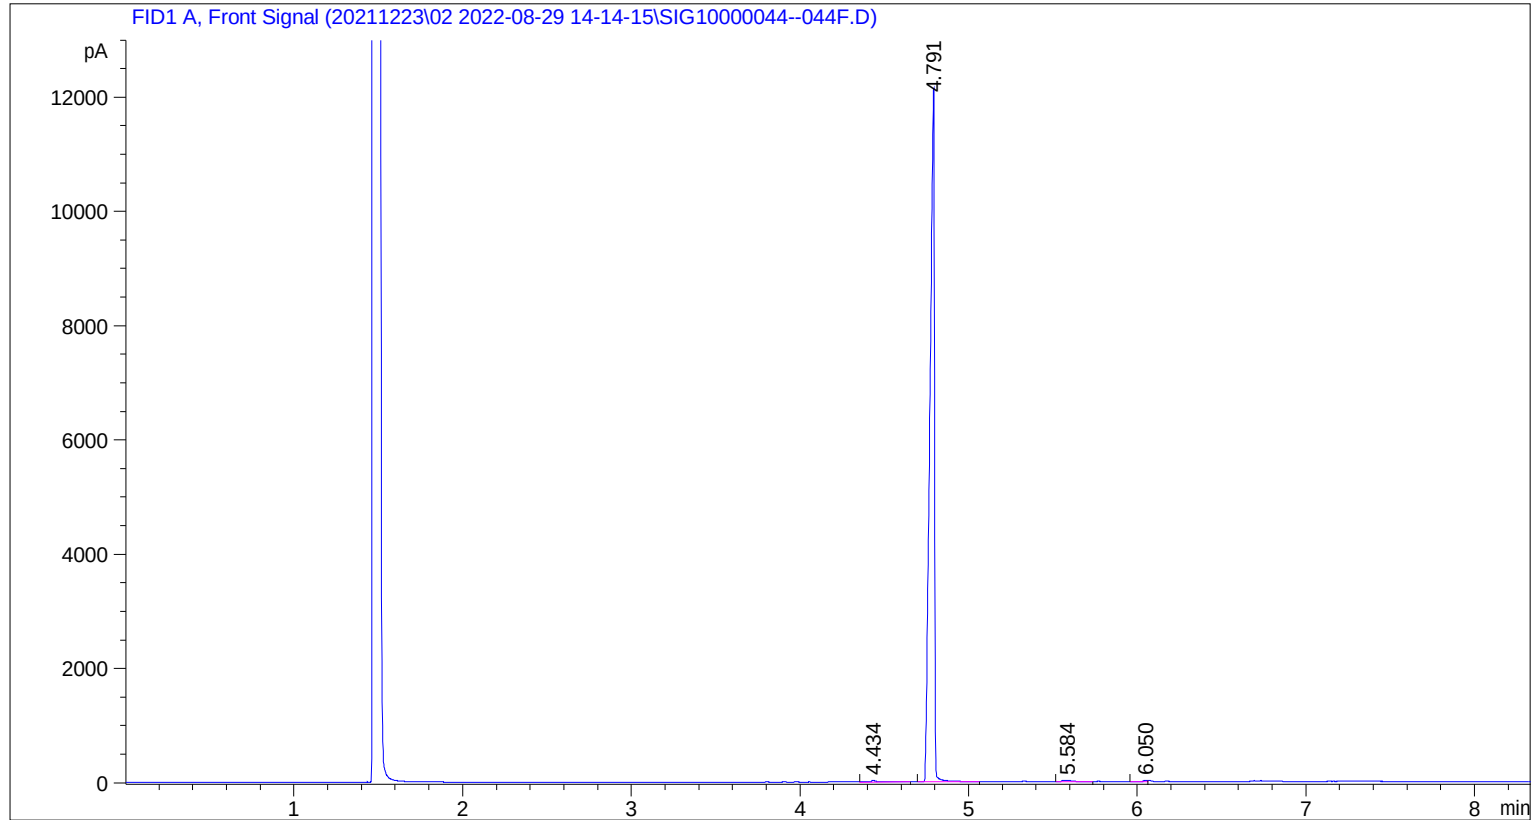

Area Percent Report

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: FID1 A, Front Signal

| Peak # | RetTime [min] | Type | Width [min] | Area [pA*s] | Height [pA] | Area %   |
|--------|---------------|------|-------------|-------------|-------------|----------|
| 1      | 4.434         | VV R | 0.0318      | 75.19354    | 31.57783    | 0.32735  |
| 2      | 4.791         | BB   | 0.0276      | 2.27476e4   | 1.23060e4   | 99.03138 |
| 3      | 5.584         | BV R | 0.0661      | 110.43302   | 22.98343    | 0.48077  |
| 4      | 6.050         | VV R | 0.0226      | 36.86697    | 24.49821    | 0.16050  |

Totals :                      2.29701e4   1.23851e4

=====  
\*\*\* End of Report \*\*\*