

Certificate of Analysis^(Ver.2.0)

Alternariol

1. General information

This document is designed and the certified value(s) and uncertainty(ies) are determined in accordance with ISO Guide 31^[1] and Eurachem / CITAC Guides^[2,3].

2. Description of the Reference Material (RM)

Product name: Alternariol

Product number: MSS1030

CAS number: 641-38-3

Formula: C₁₄H₁₀O₅

Formula weight: 258.23

Lot#: 2C0D28


Physical description of RM: Off-white to light brown powder of Alternariol

Amount: 1mg

Production date: 28, Apr, 2023

Expiry date: 27, Apr, 2026

Name of the supplier: Pribolab Pte. Ltd .
Building 21, MAX Business Hongwan, High-Tech Zone, Qingdao, China
www.pribolab.com, pribolab@gmail.com



2.1 Intended use of the RM

- for laboratory use only
- calibration of analytical instruments

2.2 Instruction for the correct use of the RM

The compound should be stored at -20°C in a dark place. Before usage of the RM, the compound should be allowed to warm to temperature (20±3°C). The recommended minimum sub-sample amount for all kinds of application is 1mg. Certified values and uncertainties can only be guaranteed if the minimum sampling volume requirement is met. The expiry date of this RM is based on the current knowledge and holds only for proper storage conditions in the originally closed flasks/packages.

2.3 Hazardous situation

The normal laboratory safety precautions should be observed when working with this RM. Further details for the handling of this RM are available as safety data sheet.

3. Certified values and their uncertainties

Alternariol		
Compound	Purity	
Alternariol	Certified value ^a	Uncertainty ^b
	99.1%	±0.9%
a The certified value is based upon the results from several analytical techniques		
b Expanded uncertainty U (k = 2) of the value u _c according to GUM ^[4]		

4. Discussion of traceability

The qualitative analysis for principal component of the material is obtained by liquid chromatography-mass spectrometry (LC-MS) and nuclear magnetic resonance (NMR). The certified value (purity of Alternariol) is based on the results of mass balance method and qNMR method. Structure related impurities are determined by liquid chromatography - tandem mass spectrometry (LC-MS/MS). Moisture content, inorganic impurities and volatile organic compounds are measured by Karl Fischer, ICP-MS and GC-FID respectively. Based on the above results, the purity certification value is given.

All weighting and dilution steps for preparation were done using calibrated equipment (microbalances, pipettes). The gravimetric preparation furthermore was performed in a standardized and certified class A flask with stated uncertainty as well as using traceable thermometers for temperature controlled preparation. The whole preparation process is therefore traceable to SI units and metrological traceability is given.

5. Purity assessment of Alternariol

5.1 HPLC-DAD


The purity check using LC-DAD of the Alternariol sample showed one main peak after blank subtraction. The peak purity of the main signal was examined by diode array spectra of the Alternariol peak and led to the conclusion that this peak consists only of Alternariol.

5.2 LC-MS/MS

The purity check using gradient LC-MS/MS of the Alternariol sample showed one main peak after blank subtraction.

6. Further information

The purchaser must determine the suitability of this product for its particular use. Pribolab makes no warranty of any kind, express or implied, other than its products meet all quality control standards set by Pribolab. We do not guarantee that the product can be used for a special application.

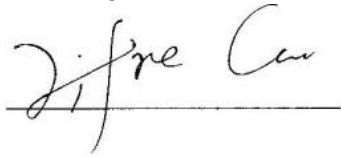

Inspected by

Quality System Specialist

References:

- [1] ISO Guide 31:2015-1-18, "Reference materials—contents of certificates, labels and accompanying documentation"
- [2] Eurachem / CITAC Guide, 1-37, (2003), "Traceability in Chemical Measurement"
- [3] Eurachem / CITAC Guide CG4, 1-133, (QUAM:2012.P1), "Quantifying Uncertainty in Analytical Measurement", 3rd Ed.
- [4] International Organization for Standardization (ISO), (1995), "Guide to the Expression of Uncertainty in Measurement", 1st Ed. Geneva, Switzerland